
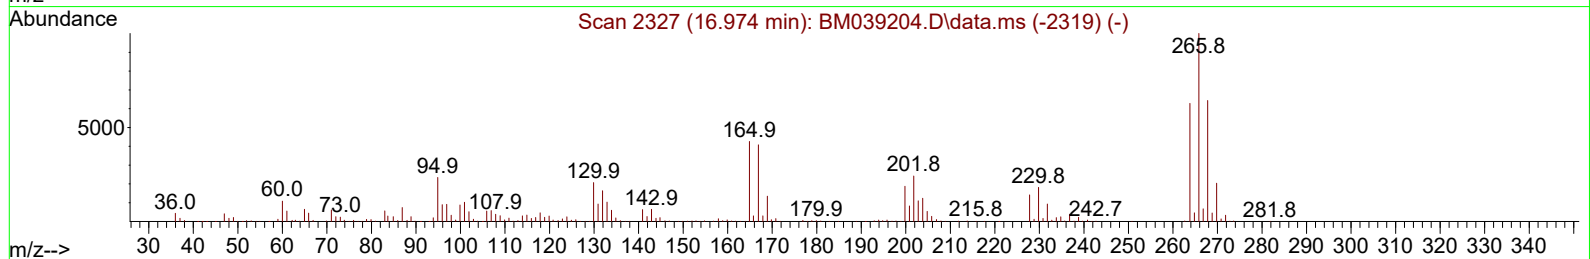
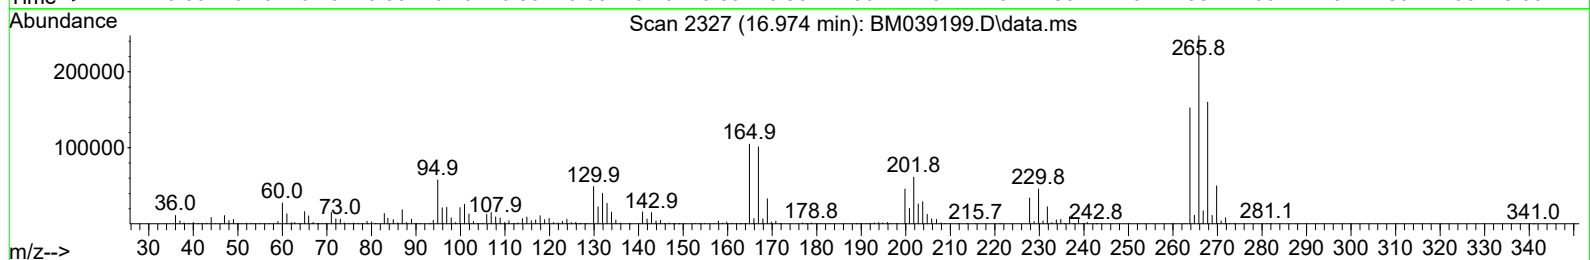


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032923\
Data File : BM039199.D
Acq On : 29 Mar 2023 11:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 30 06:50:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 30 05:15:45 2023
Response via : Initial Calibration

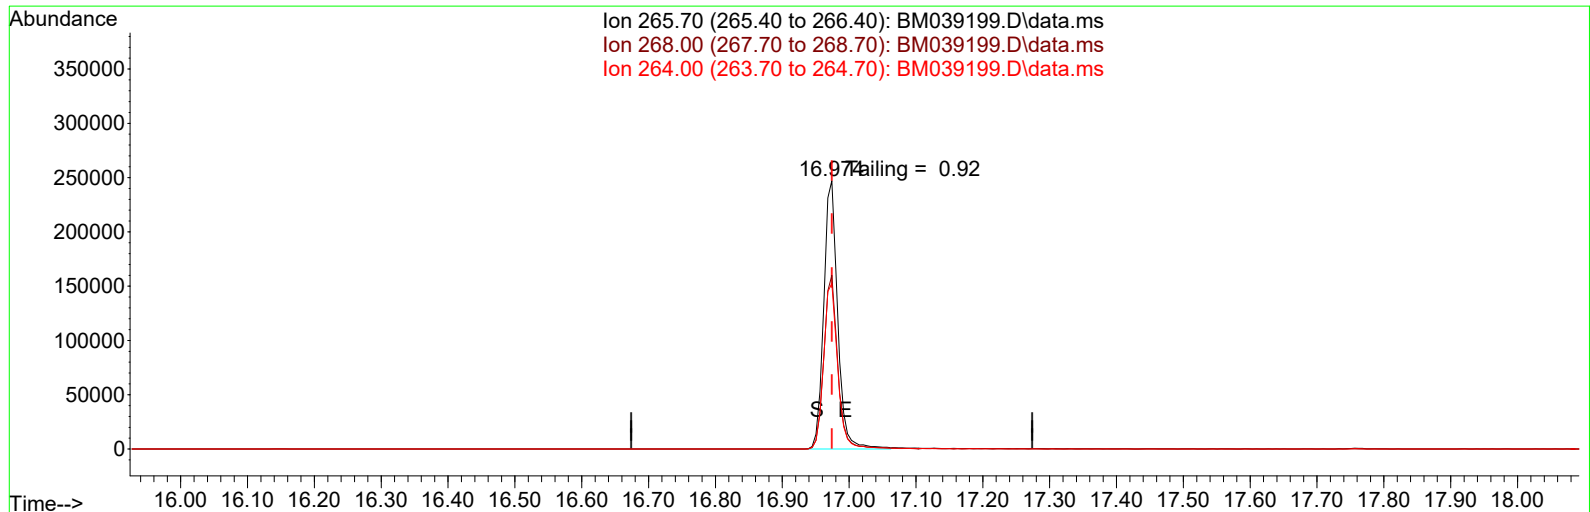

TIC: BM039199.D\data.ms

(70) Pentachlorophenol (C)




16.974min (-0.000) 0.00 ng

response 359458

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	64.72
264.00	62.80	61.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032923\
Data File : BM039199.D
Acq On : 29 Mar 2023 11:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 30 06:50:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 30 05:15:45 2023
Response via : Initial Calibration

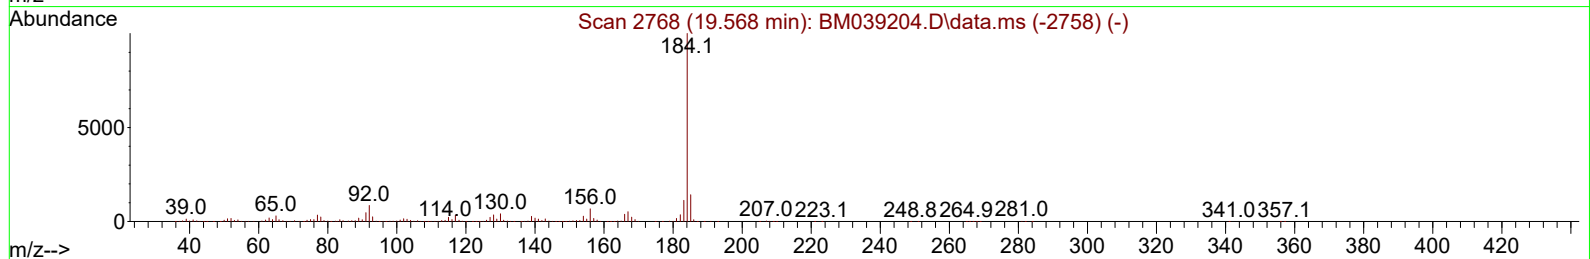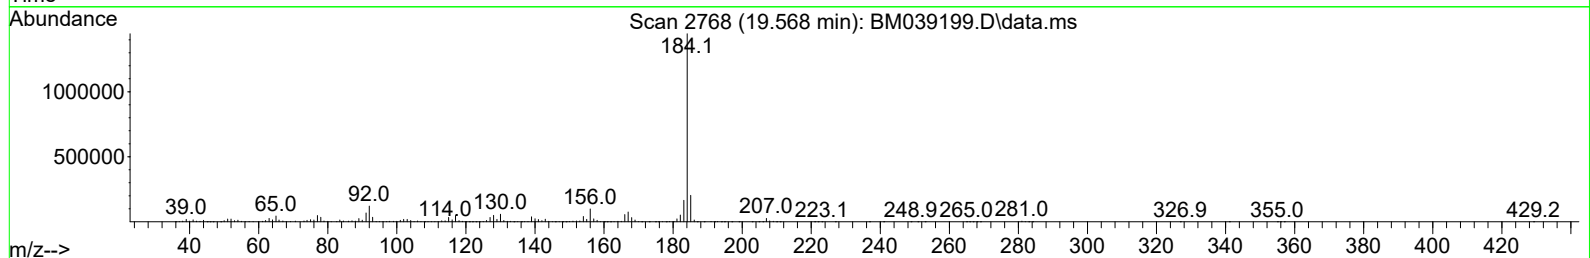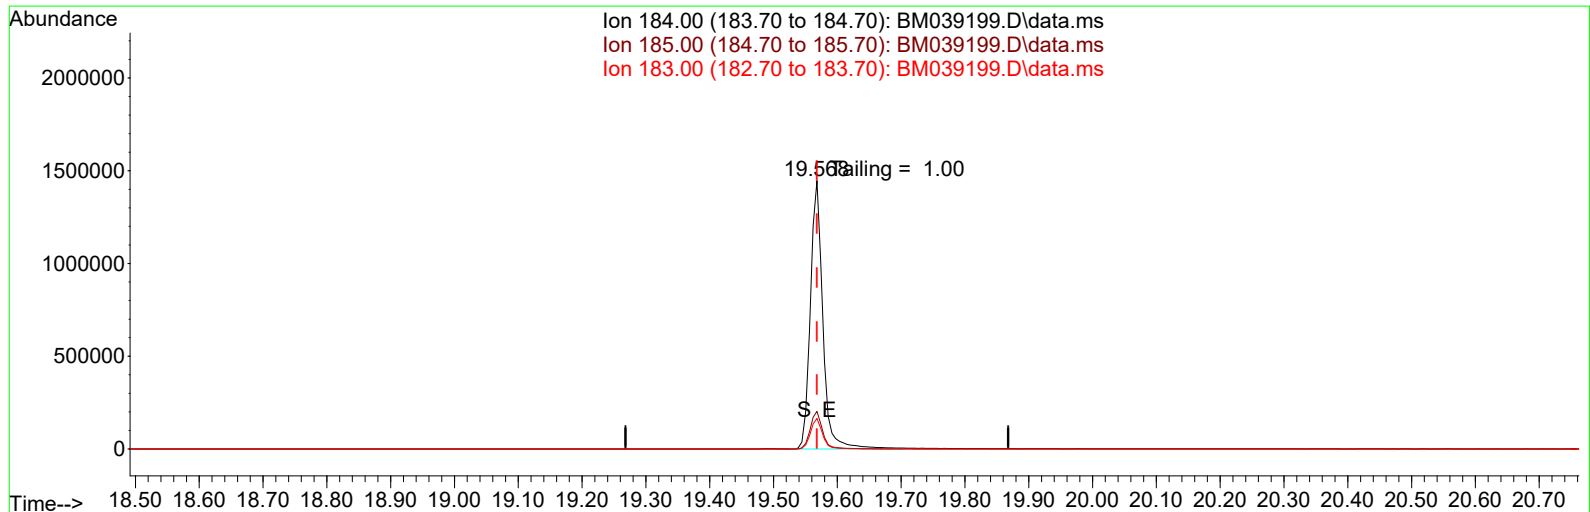

TIC: BM039199.D\data.ms

(77) Benzidine**19.568min (-0.000) 344269.27 ng****response 1988649**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.02
183.00	11.20	11.38
0.00	0.00	0.00