

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032923\
 Data File : BM039215.D
 Acq On : 29 Mar 2023 21:32
 Operator : CG/JU
 Sample : PB151721BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB151721BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM039215.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.016	288	294	305	rBV	1894094	2528943	25.95%	4.794%
2	5.487	367	374	385	rBV	4565039	6371263	65.39%	12.077%
3	7.092	640	647	663	rBV	4073955	6298822	64.65%	11.940%
4	7.928	782	789	798	rBV	730212	1156416	11.87%	2.192%
5	9.092	980	987	1009	rBV	2453053	4051652	41.58%	7.680%
6	10.739	1259	1267	1281	rBV	857712	1518318	15.58%	2.878%
7	13.198	1677	1685	1700	rBV	5537921	8221493	84.38%	15.584%
8	14.568	1909	1918	1933	rBV	1180031	1770525	18.17%	3.356%
9	16.062	2165	2172	2191	rBV	3650758	5419930	55.63%	10.274%
10	17.315	2379	2385	2400	rBV	1273176	1886391	19.36%	3.576%
11	19.939	2826	2831	2842	rBV	7780338	9743616	100.00%	18.469%
12	21.503	3092	3097	3105	rBV	1338937	1859321	19.08%	3.524%
13	23.915	3502	3507	3517	rVB2	941092	1928844	19.80%	3.656%




Sum of corrected areas: 52755534

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032923\
Data File : BM039215.D
Acq On : 29 Mar 2023 21:32
Operator : CG/JU
Sample : PB151721BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB151721BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

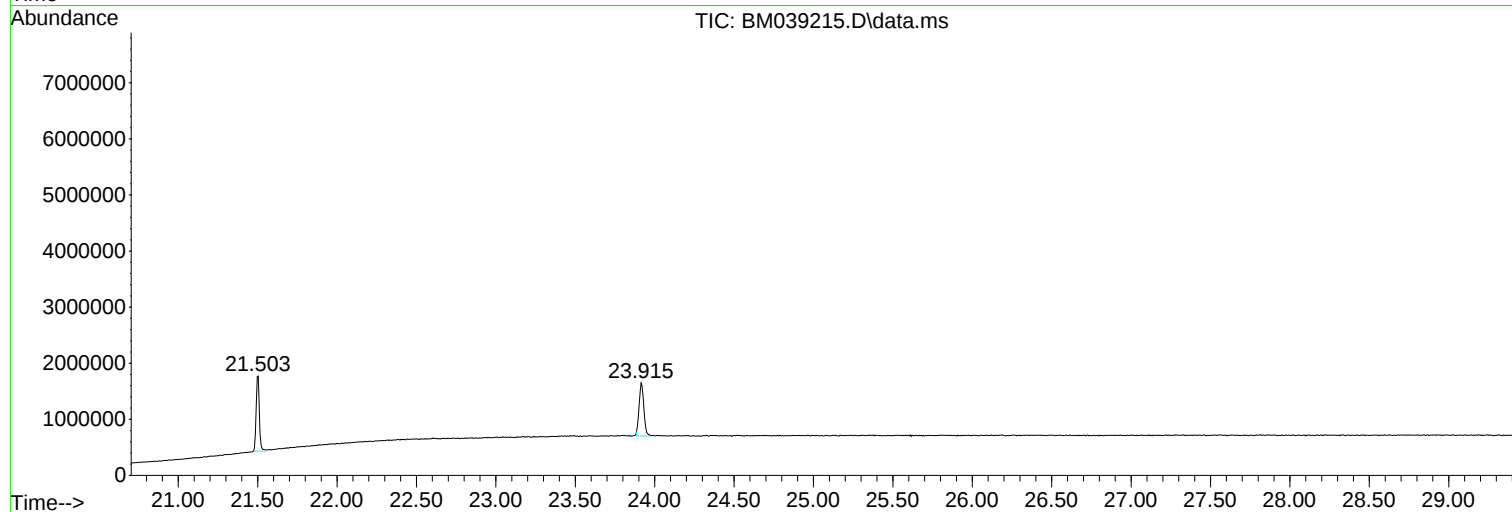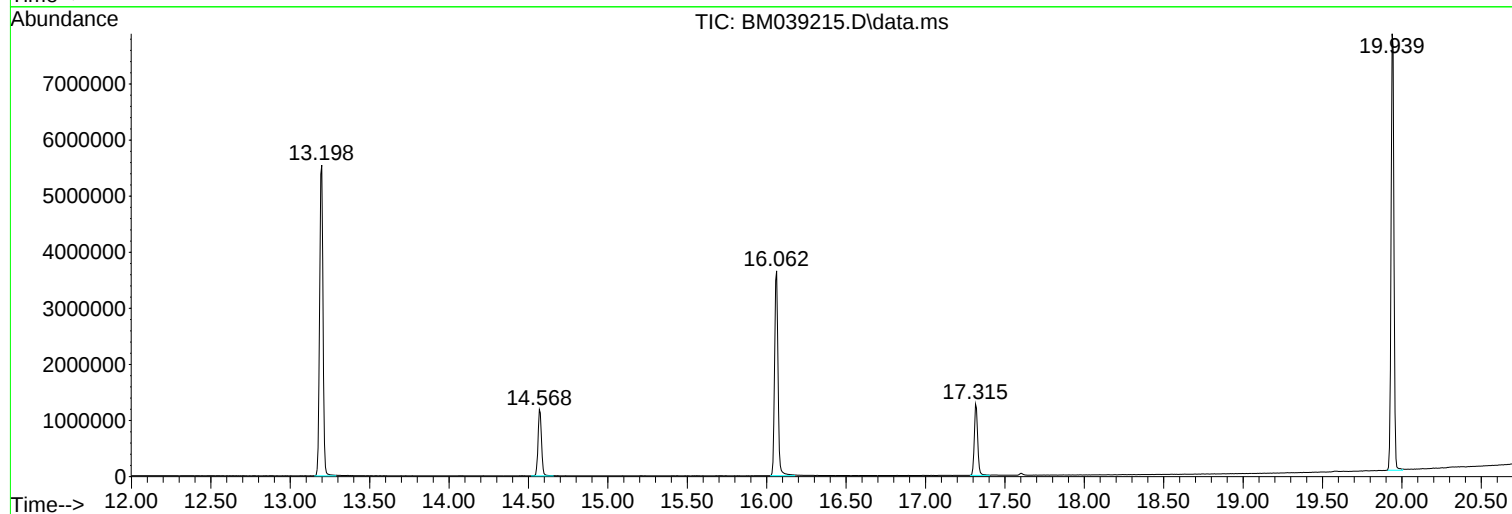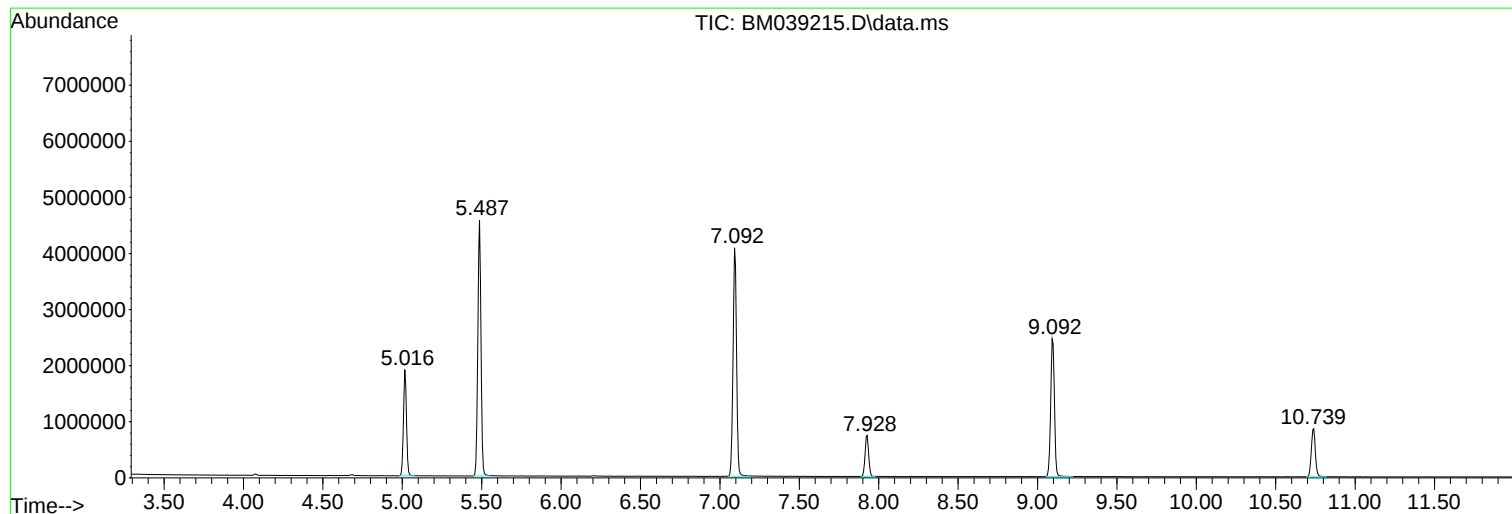

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032923\
Data File : BM039215.D
Acq On : 29 Mar 2023 21:32
Operator : CG/JU
Sample : PB151721BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB151721BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.016	43.74 ng	2528940	1,4-Dichlorobenzene-d4	7.928

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56		
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23		
3	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	17		
4	5-Hexen-2-one	98	C6H10O	000109-49-9	9		
5	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9		

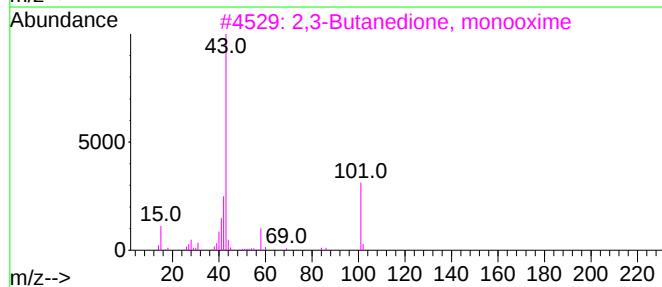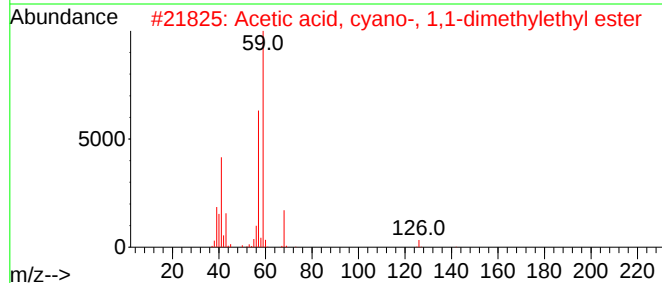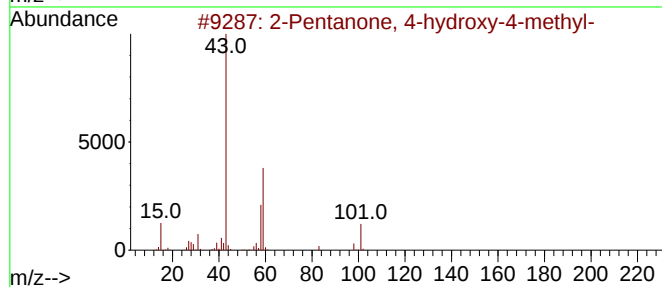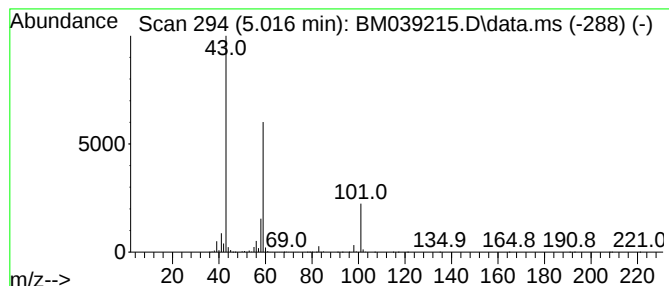

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032923\
Data File : BM039215.D
Acq On : 29 Mar 2023 21:32
Operator : CG/JU
Sample : PB151721BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB151721BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.016	43.7	ng	2528940	1	7.928	1156420	20.0