
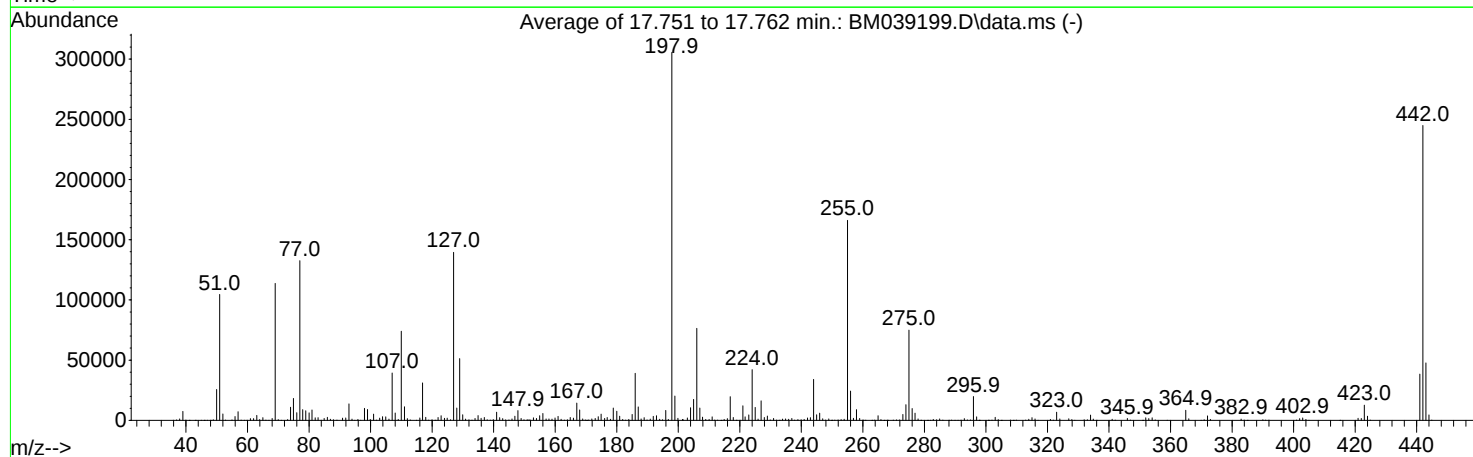


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032923\
Data File : BM039199.D
Acq On : 29 Mar 2023 11:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 30 05:15:45 2023

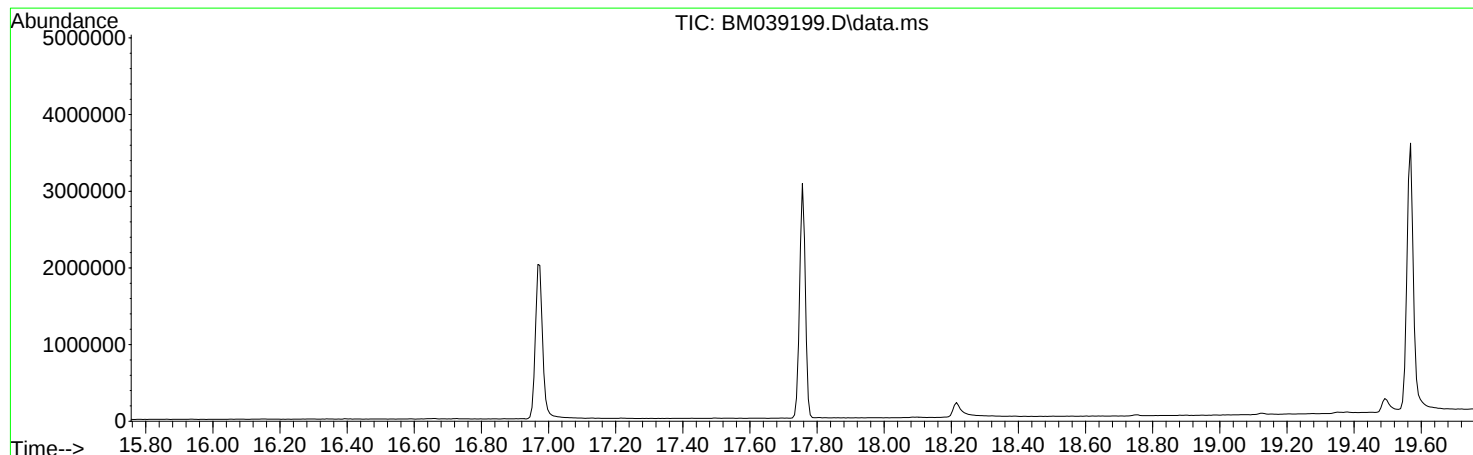




AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2452

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.2	104551	PASS
68	69	0.00	2	1.4	1624	PASS
69	198	0.00	100	37.2	113709	PASS
70	69	0.00	2	0.6	712	PASS
127	198	10	80	45.7	139584	PASS
197	198	0.00	2	0.3	879	PASS
198	198	100	100	100.0	305493	PASS
199	198	5	9	6.6	20189	PASS
275	198	10	60	24.5	74992	PASS
365	198	1	100	2.8	8404	PASS
441	198	0.01	100	12.6	38405	PASS
442	442	50	100	100.0	244971	PASS
443	442	15	24	19.5	47747	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032923\
Data File : BM039199.D
Acq On : 29 Mar 2023 11:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 30 06:50:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 30 05:15:45 2023
Response via : Initial Calibration

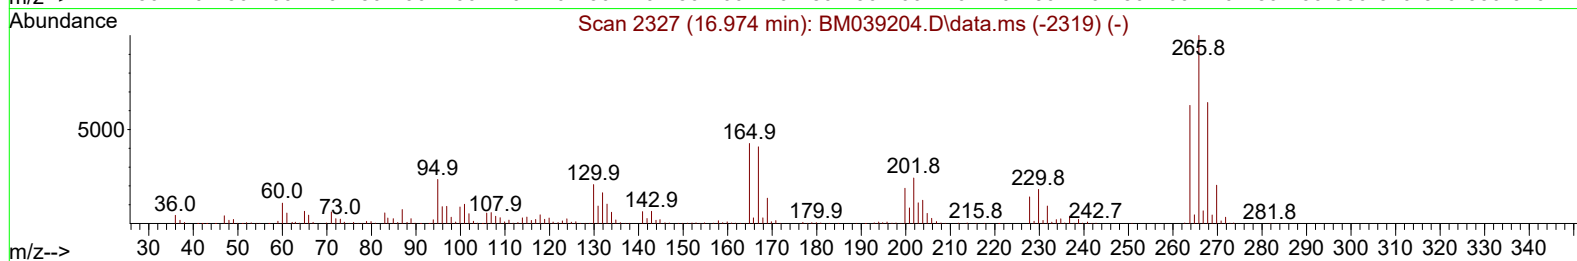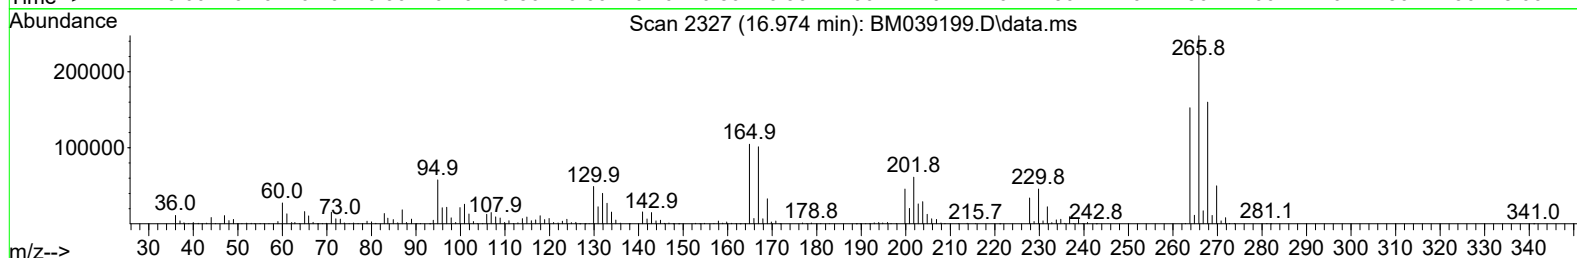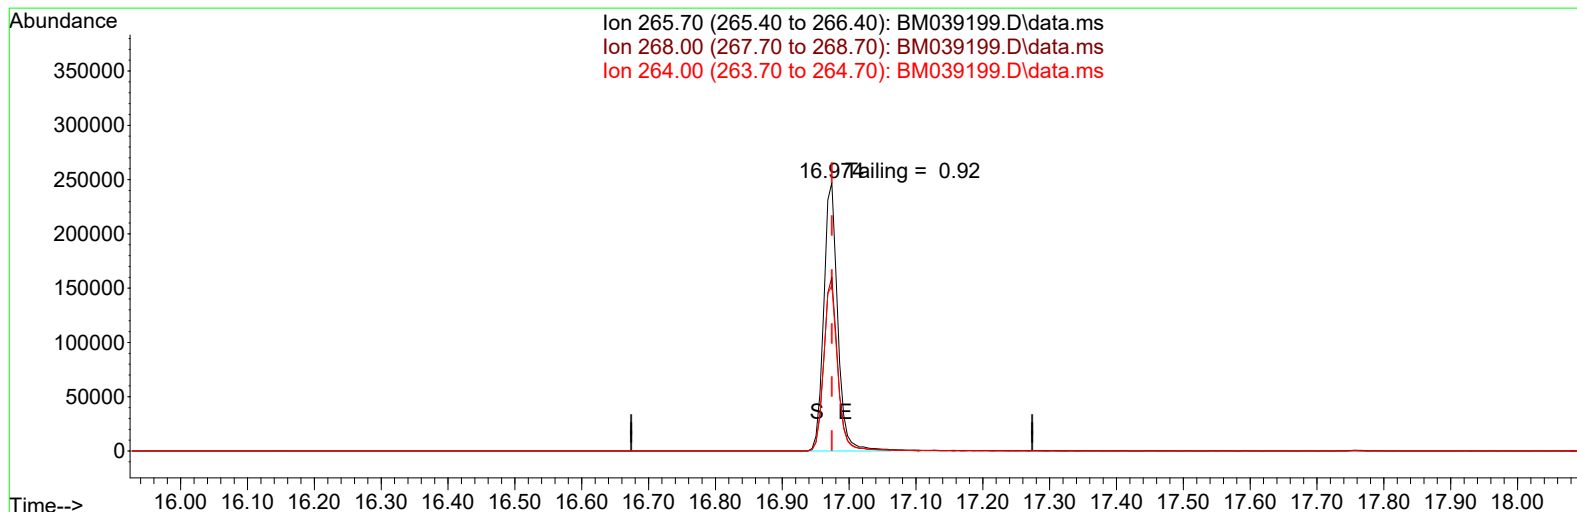

TIC: BM039199.D\data.ms

(70) Pentachlorophenol (C)

16.974min (-0.000) 0.00 ng




response 359458

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	64.72
264.00	62.80	61.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032923\
 Data File : BM039199.D
 Acq On : 29 Mar 2023 11:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Mar 30 06:50:36 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 30 05:15:45 2023
 Response via : Initial Calibration

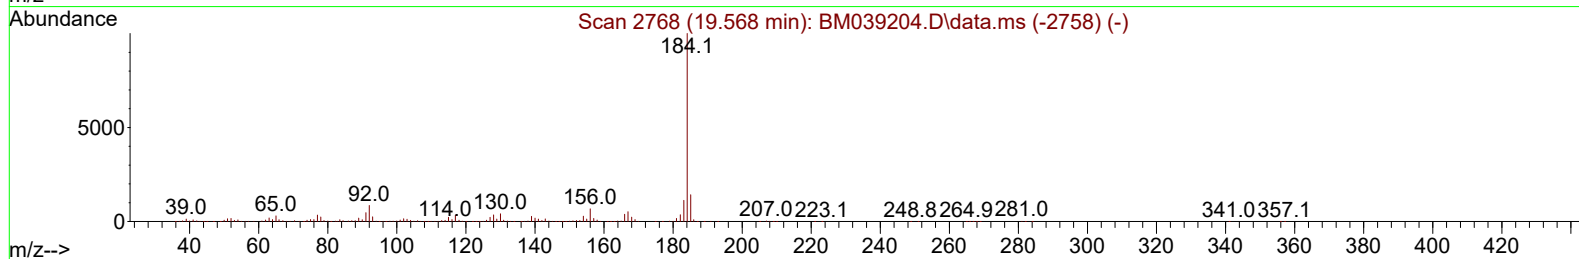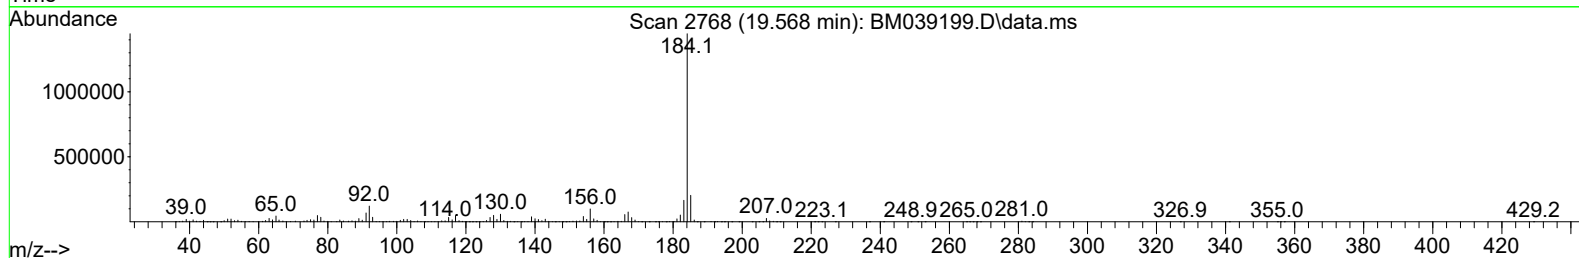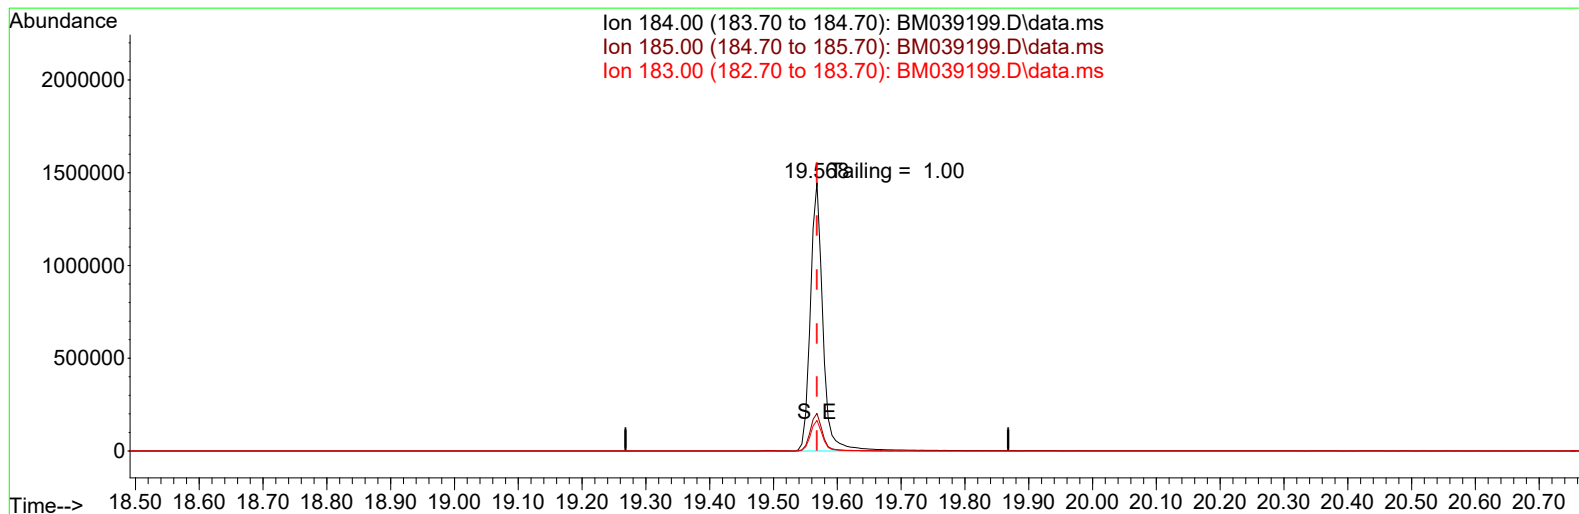

TIC: BM039199.D\data.ms

(77) Benzidine**19.568min (-0.000) 344269.27 ng****response 1988649**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.02
183.00	11.20	11.38
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/29/2023	BNA_M	<u>BM039199.D</u>
Compound Name	Response	Retention Time
DDT	1071237	20.797
DDD	15742	20.409
DDE	291	19.85
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16033	1087270	1.47

Instrument :
BNA_M
ClientSampleId :
DFTPP