

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM033019\
 Data File : BM019618.D
 Acq On : 30 Mar 2019 14:23
 Operator : JU/SJ
 Sample : K2065-11
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF5L4

Manual Integrations
 APPROVED

Sohil
 4/1/2019 5:50:48 PM

Quant Time: Mar 30 21:53:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 29 14:33:17 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	121561	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	548550	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.23	164	312940	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.99	188	705506	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	861765	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	1055981	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	16878	5.44	ng/uL	0.00
5) Phenol-d5	6.76	99	177376	16.39	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	120186	16.58	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	143234	17.46	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	121274	14.92	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	67762	17.32	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	74888	17.20	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	126402	15.38	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	167116	16.93	ng/ul	0.00
44) Dimethylphthalate-d6	13.66	166	466530	18.48	ng/ul	0.00
47) Acenaphthylene-d8	13.93	160	534660	16.93	ng/ul	0.00
52) 4-Nitrophenol-d4	14.50	143	44605m	11.27	ng/ul	0.02
58) Fluorene-d10	15.24	176	391905	18.01	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	38075	8.16	ng/ul	0.00
71) Anthracene-d10	17.09	188	608101	17.96	ng/ul	0.00
79) Pyrene-d10	19.40	212	686368	17.24	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.27	264	900735	16.09	ng/ul	0.00

Target Compounds					Qvalue
45) Dimethylphthalate	13.70	163	65879	2.600 ng/ul#	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM033019\
Data File : BM019618.D
Acq On : 30 Mar 2019 14:23
Operator : JU/SJ
Sample : K2065-11
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampled :
BF5L4

Quant Time: Mar 30 21:53:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 29 14:33:17 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
4/1/2019 5:50:48 PM

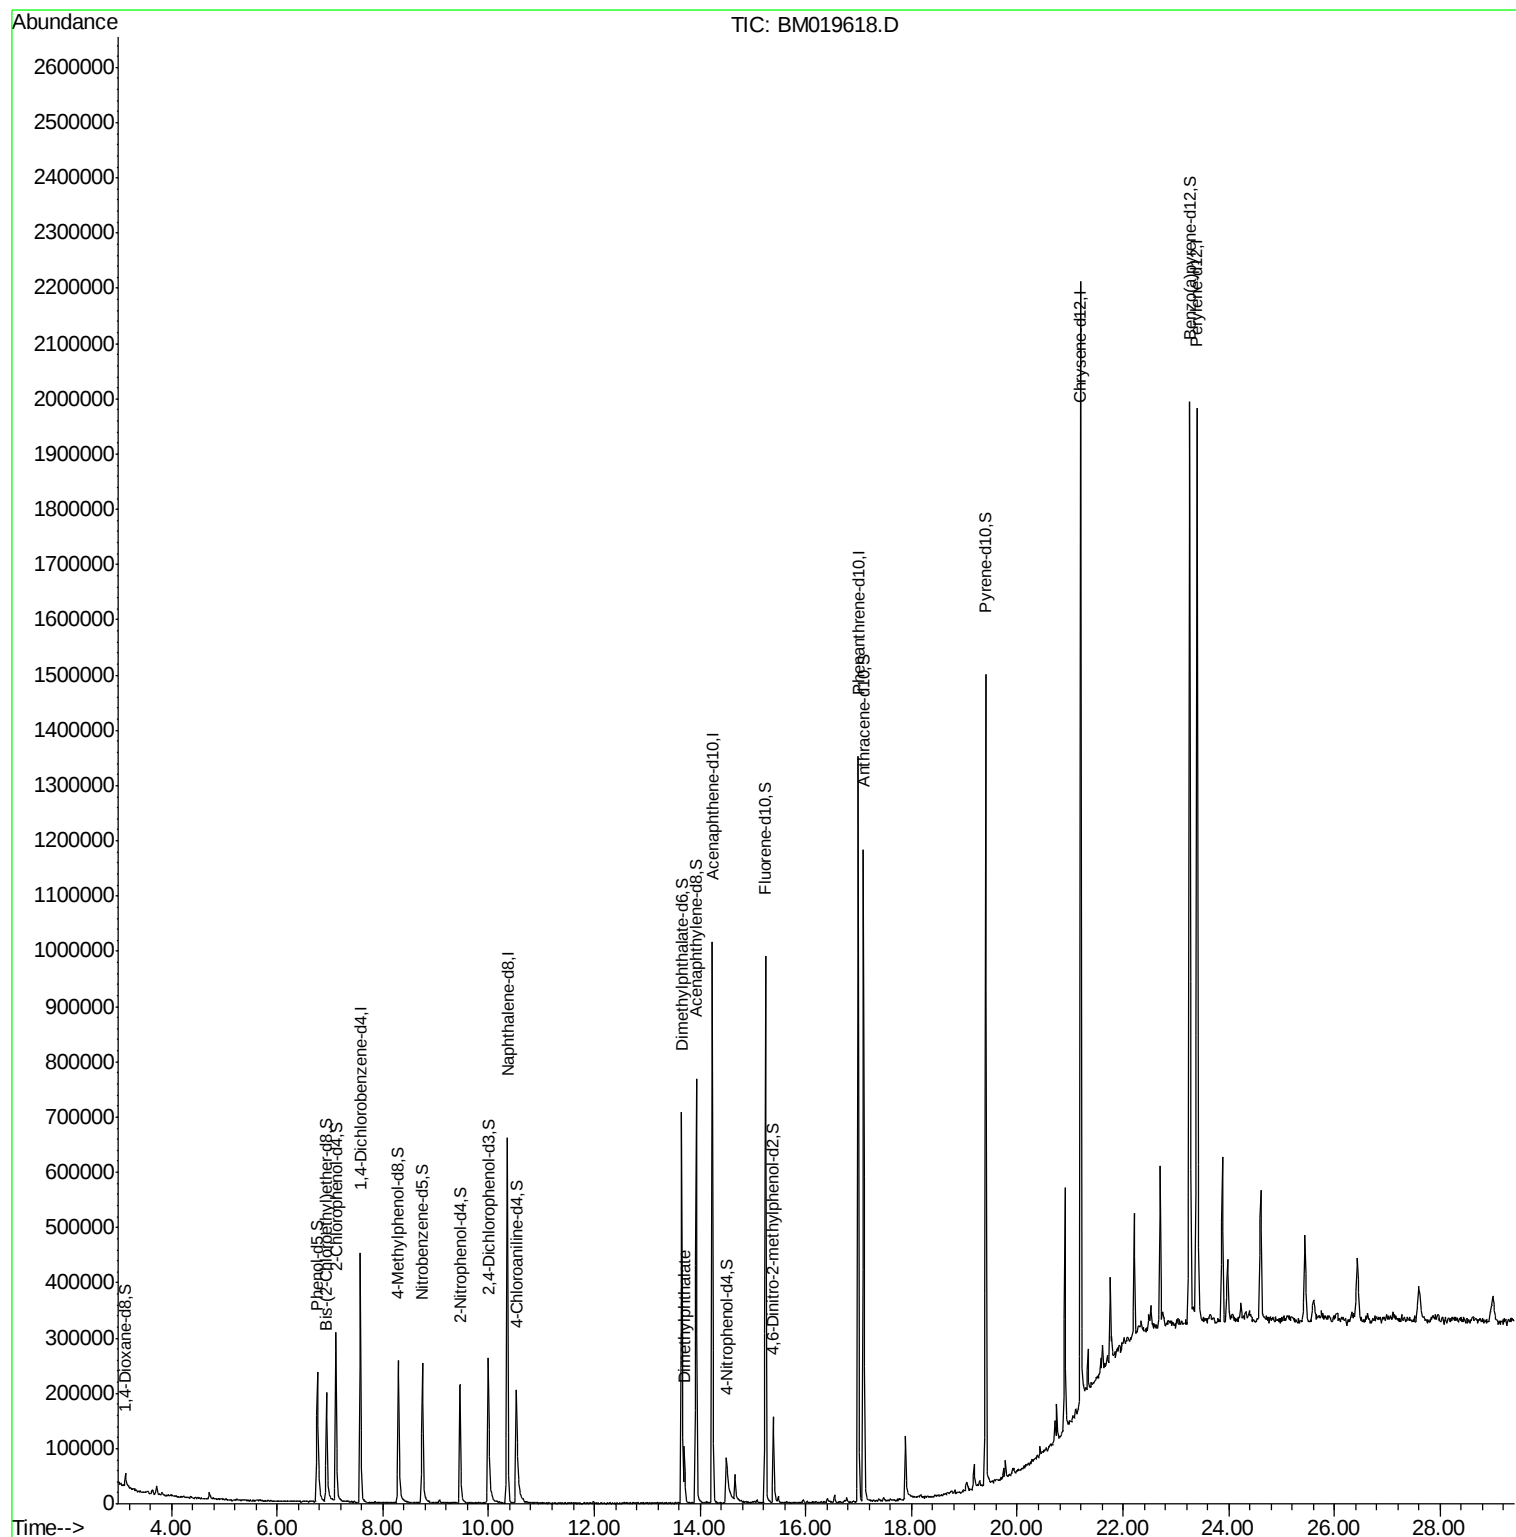

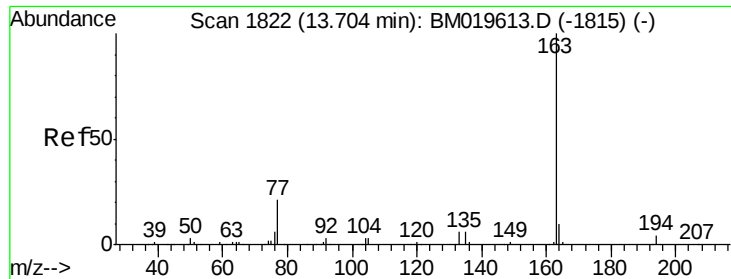

#45
 Dimethylphthalate
 Concen: 2.600 ng/ul
 RT: 13.70 min Scan# 1822
 Delta R.T. -0.01 min
 Lab File: BM019618.D
 Acq: 30 Mar 2019 14:23

Instrument :
 BNA_M
 ClientSampleId :
 BF5L4

Tgt Ion	Ratio	Resp Lower	Upper
163	100		
194	3.7	4.0	6.0#
164	9.0	8.4	12.6

Manual Integrations
 APPROVED

Sohil
 4/1/2019 5:50:48 PM

