

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM033019\
 Data File : BM019619.D
 Acq On : 30 Mar 2019 14:59
 Operator : JU/SJ
 Sample : K2065-18
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF5L7

Manual Integrations
 APPROVED

Sohil
 4/1/2019 5:50:49 PM

Quant Time: Mar 30 21:59:28 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 29 14:33:17 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	137223	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	611050	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.23	164	343882	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.99	188	766968	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	964233	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	1165874	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	17128	4.89	ng/uL	0.00
5) Phenol-d5	6.76	99	196783	16.10	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	141674	17.32	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	161947	17.49	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	145634	15.88	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	75732	17.37	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	83024	17.11	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	143826	15.71	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	172173	15.66	ng/ul	0.00
44) Dimethylphthalate-d6	13.66	166	492080	17.73	ng/ul	0.00
47) Acenaphthylene-d8	13.93	160	578774	16.68	ng/ul	0.00
52) 4-Nitrophenol-d4	14.50	143	54458m	12.52	ng/ul	0.02
58) Fluorene-d10	15.23	176	426370	17.84	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	47305	9.33	ng/ul	0.00
71) Anthracene-d10	17.09	188	643718	17.49	ng/ul	0.00
79) Pyrene-d10	19.40	212	731112	16.42	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	967702	15.66	ng/ul	0.00

Target Compounds					Qvalue
45) Dimethylphthalate	13.70	163	71977	2.585 ng/ul#	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM033019\
Data File : BM019619.D
Acq On : 30 Mar 2019 14:59
Operator : JU/SJ
Sample : K2065-18
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BF5L7

Quant Time: Mar 30 21:59:28 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 29 14:33:17 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
4/1/2019 5:50:49 PM

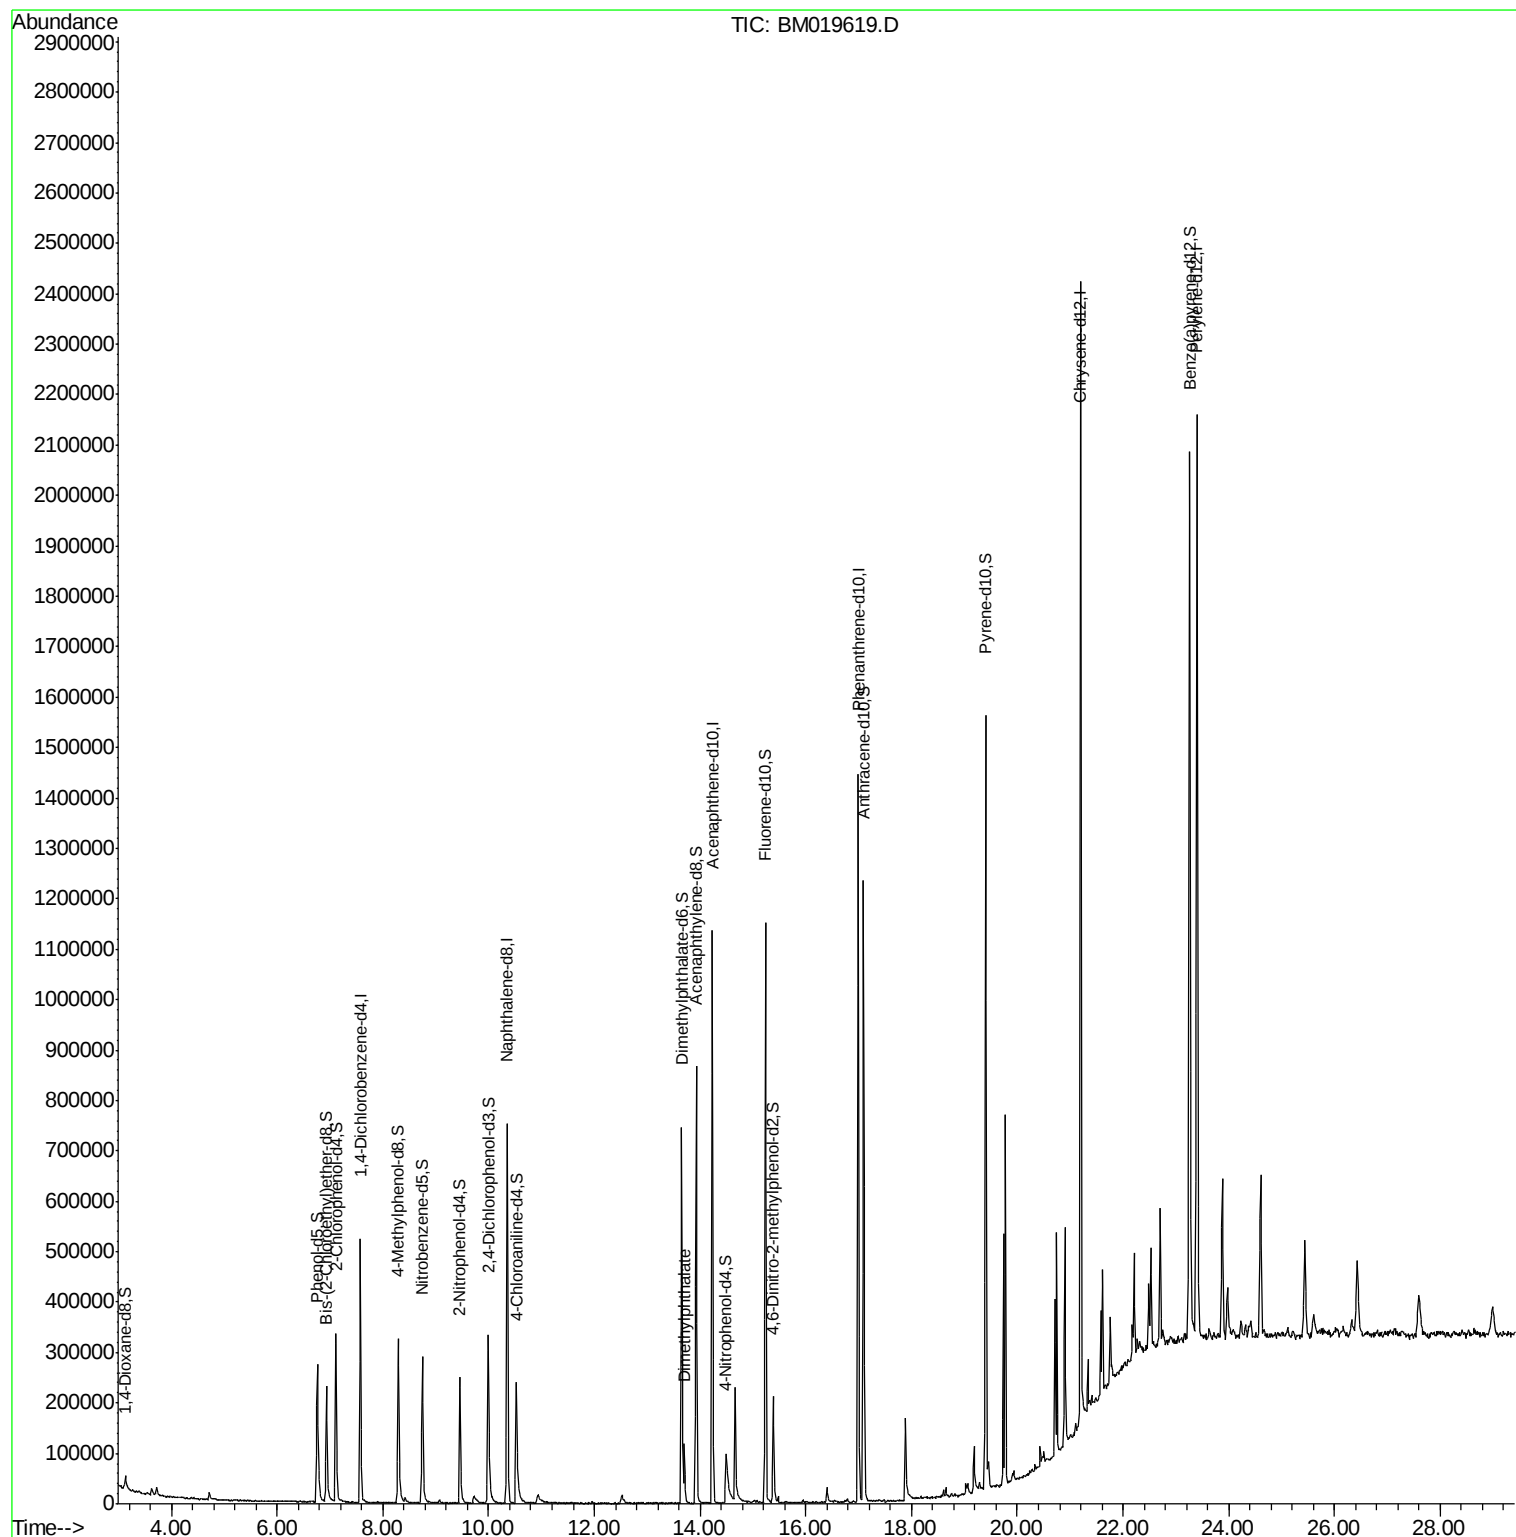

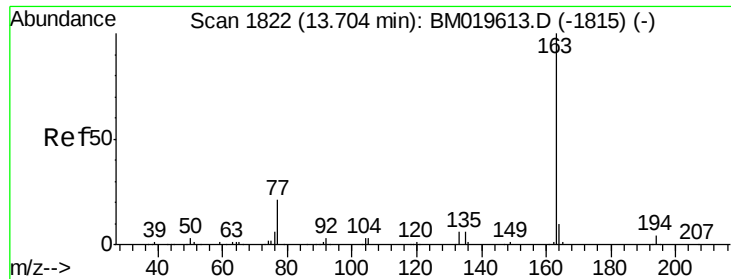

#45
 Dimethylphthalate
 Concen: 2.585 ng/ul
 RT: 13.70 min Scan# 1822
 Delta R.T. -0.01 min
 Lab File: BM019619.D
 Acq: 30 Mar 2019 14:59

Instrument :
 BNA_M
 ClientSampleId :
 BF5L7

Tgt Ion	Ratio	Lower	Upper
163	100		
194	3.9	4.0	6.0#
164	9.7	8.4	12.6

Manual Integrations
 APPROVED

Sohil
 4/1/2019 5:50:49 PM

