

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM033019\
 Data File : BM019622.D
 Acq On : 30 Mar 2019 16:49
 Operator : JU/SJ
 Sample : K2084-21
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF7W3

Manual Integrations
 APPROVED

Sohil
 4/1/2019 5:50:50 PM

Quant Time: Mar 30 22:11:22 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 29 14:33:17 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	129889	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	583202	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.23	164	330892	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.99	188	757430	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	966545	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	1189819	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	16024	4.83	ng/uL	0.00
5) Phenol-d5	6.76	99	141593	12.24	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	103477	13.36	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	117314	13.38	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	90167	10.39	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	54445	13.09	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	61803	13.35	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.00	165	98692	11.30	ng/ul	0.00
29) 4-Chloroaniline-d4	10.53	131	103006	9.82	ng/ul	0.00
44) Dimethylphthalate-d6	13.66	166	375813	14.08	ng/ul	0.00
47) Acenaphthylene-d8	13.93	160	429364	12.86	ng/ul	0.00
52) 4-Nitrophenol-d4	14.50	143	39616m	9.47	ng/ul	0.02
58) Fluorene-d10	15.23	176	316557	13.76	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	39053	7.80	ng/ul	0.00
71) Anthracene-d10	17.09	188	490625	13.50	ng/ul	0.00
79) Pyrene-d10	19.40	212	558461	12.51	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	740321	11.74	ng/ul	0.00

Target Compounds					Qvalue
45) Dimethylphthalate	13.70	163	48801	1.822 ng/ul	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM033019\
Data File : BM019622.D
Acq On : 30 Mar 2019 16:49
Operator : JU/SJ
Sample : K2084-21
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BF7W3

Quant Time: Mar 30 22:11:22 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 29 14:33:17 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
4/1/2019 5:50:50 PM

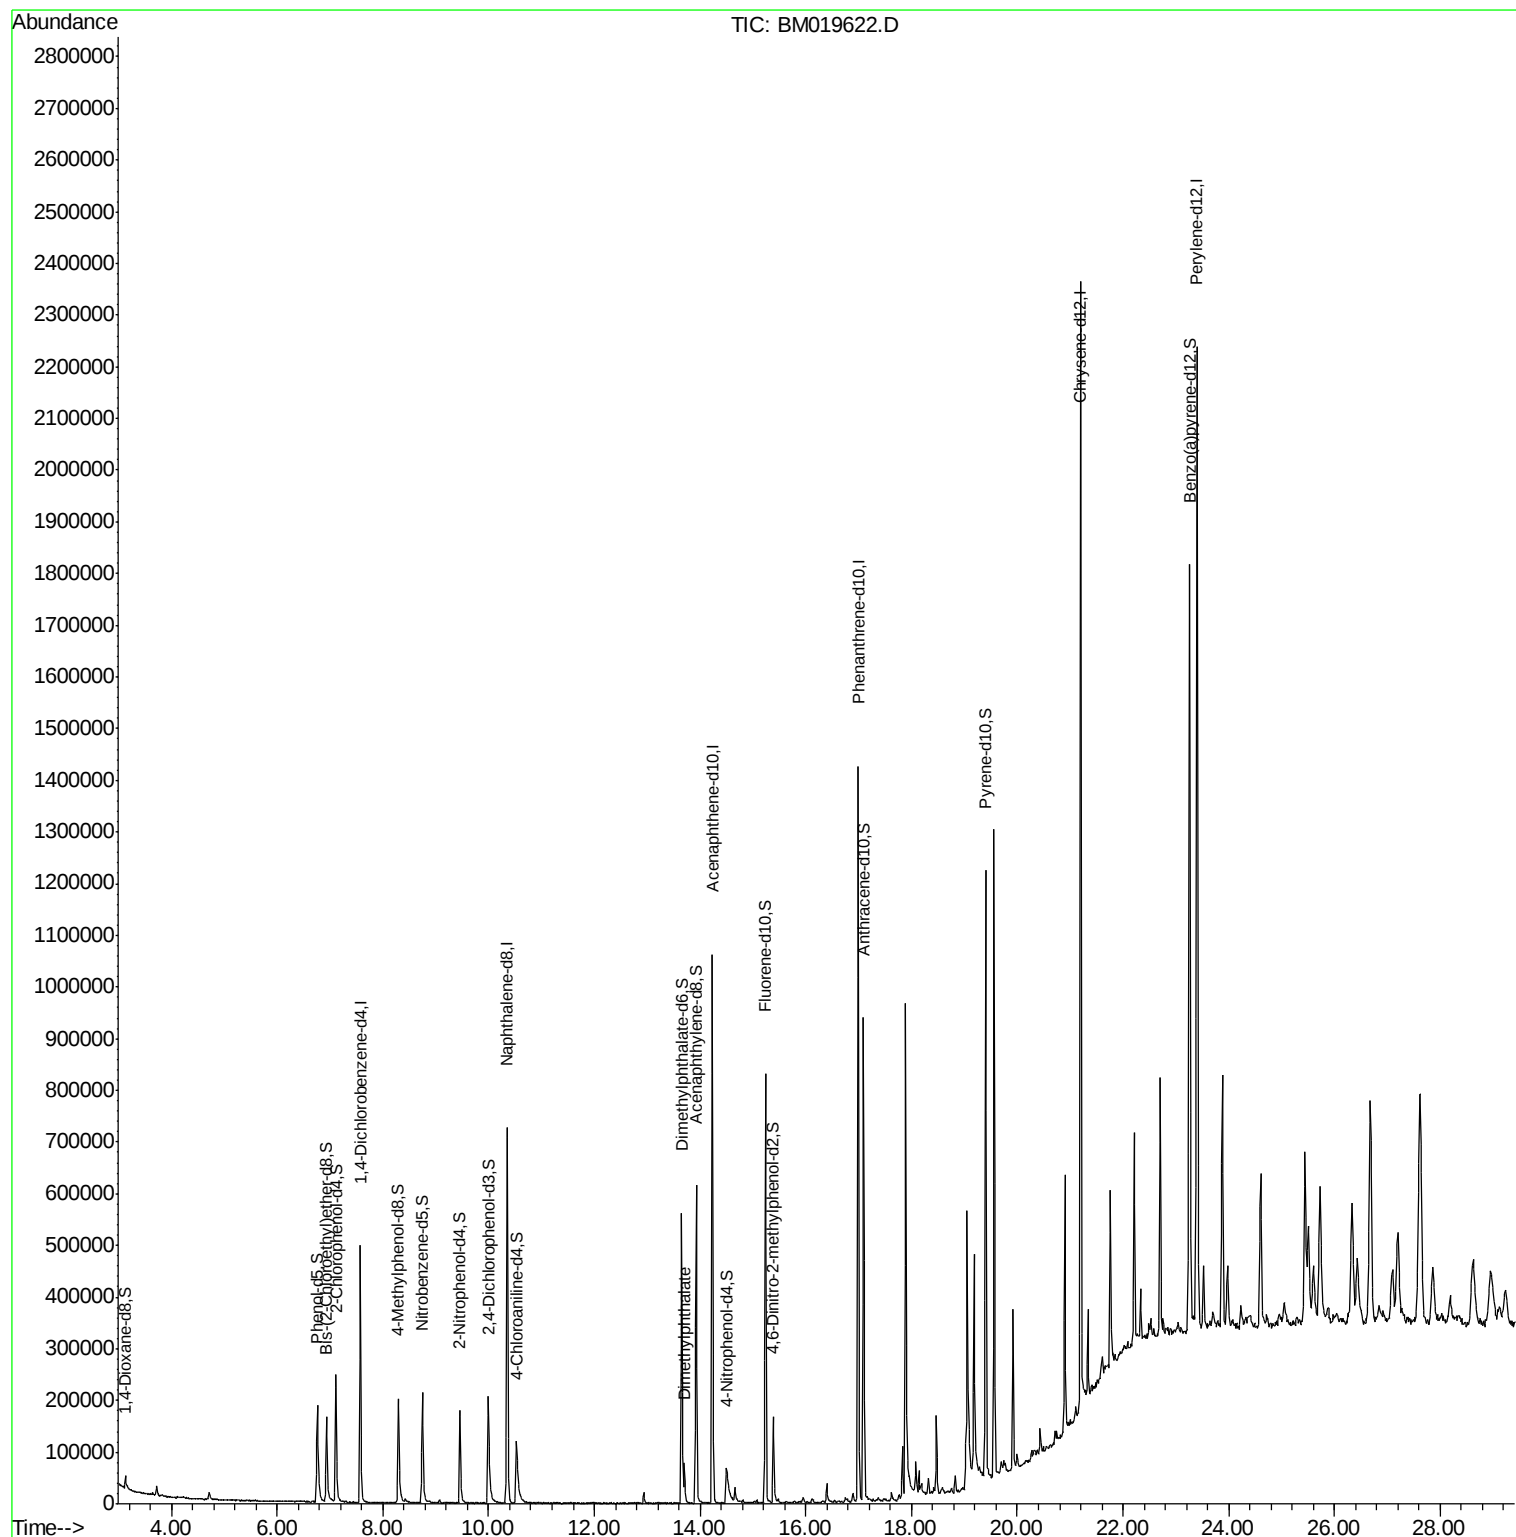

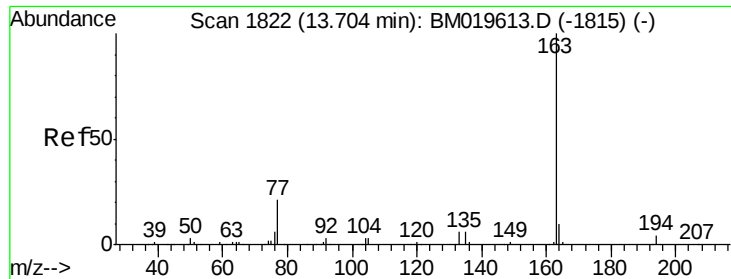

#45
 Dimethylphthalate
 Concen: 1.822 ng/ul
 RT: 13.70 min Scan# 1822
 Delta R.T. -0.01 min
 Lab File: BM019622.D
 Acq: 30 Mar 2019 16:49

Instrument :
 BNA_M
 ClientSampleId :
 BF7W3

Tgt Ion	Ratio	Resp Lower	Upper
163	100		
194	5.1	4.0	6.0
164	10.4	8.4	12.6

Manual Integrations
 APPROVED

Sohil
 4/1/2019 5:50:50 PM

