

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM033019\
 Data File : BM019623.D
 Acq On : 30 Mar 2019 17:26
 Operator : JU/SJ
 Sample : K2065-10
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF5L3

Quant Time: Mar 30 21:32:08 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 29 14:33:17 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	144696	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	629760	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.23	164	355405	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.99	188	806804	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	1004380	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	1192424	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.12	96	21559	5.83	ng/uL	0.00
5) Phenol-d5	6.76	99	210335	16.32	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	147753	17.13	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	173501	17.77	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	150969	15.61	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	78575	17.49	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	90470	18.09	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	154477	16.37	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	195750	17.28	ng/ul	0.00
44) Dimethylphthalate-d6	13.66	166	531773	18.54	ng/ul	0.00
47) Acenaphthylene-d8	13.93	160	616779	17.20	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	58560	13.03	ng/ul	0.01
58) Fluorene-d10	15.23	176	458438	18.55	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	49004	9.18	ng/ul	0.00
71) Anthracene-d10	17.09	188	706848	18.26	ng/ul	0.00
79) Pyrene-d10	19.40	212	802408	17.30	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	1035672	16.38	ng/ul	0.00


Target Compounds					Qvalue
45) Dimethylphthalate	13.70	163	78566	2.731	ng/ul# 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM033019\
Data File : BM019623.D
Acq On : 30 Mar 2019 17:26
Operator : JU/SJ
Sample : K2065-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF5L3

Quant Time: Mar 30 21:32:08 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 29 14:33:17 2019
Response via : Initial Calibration

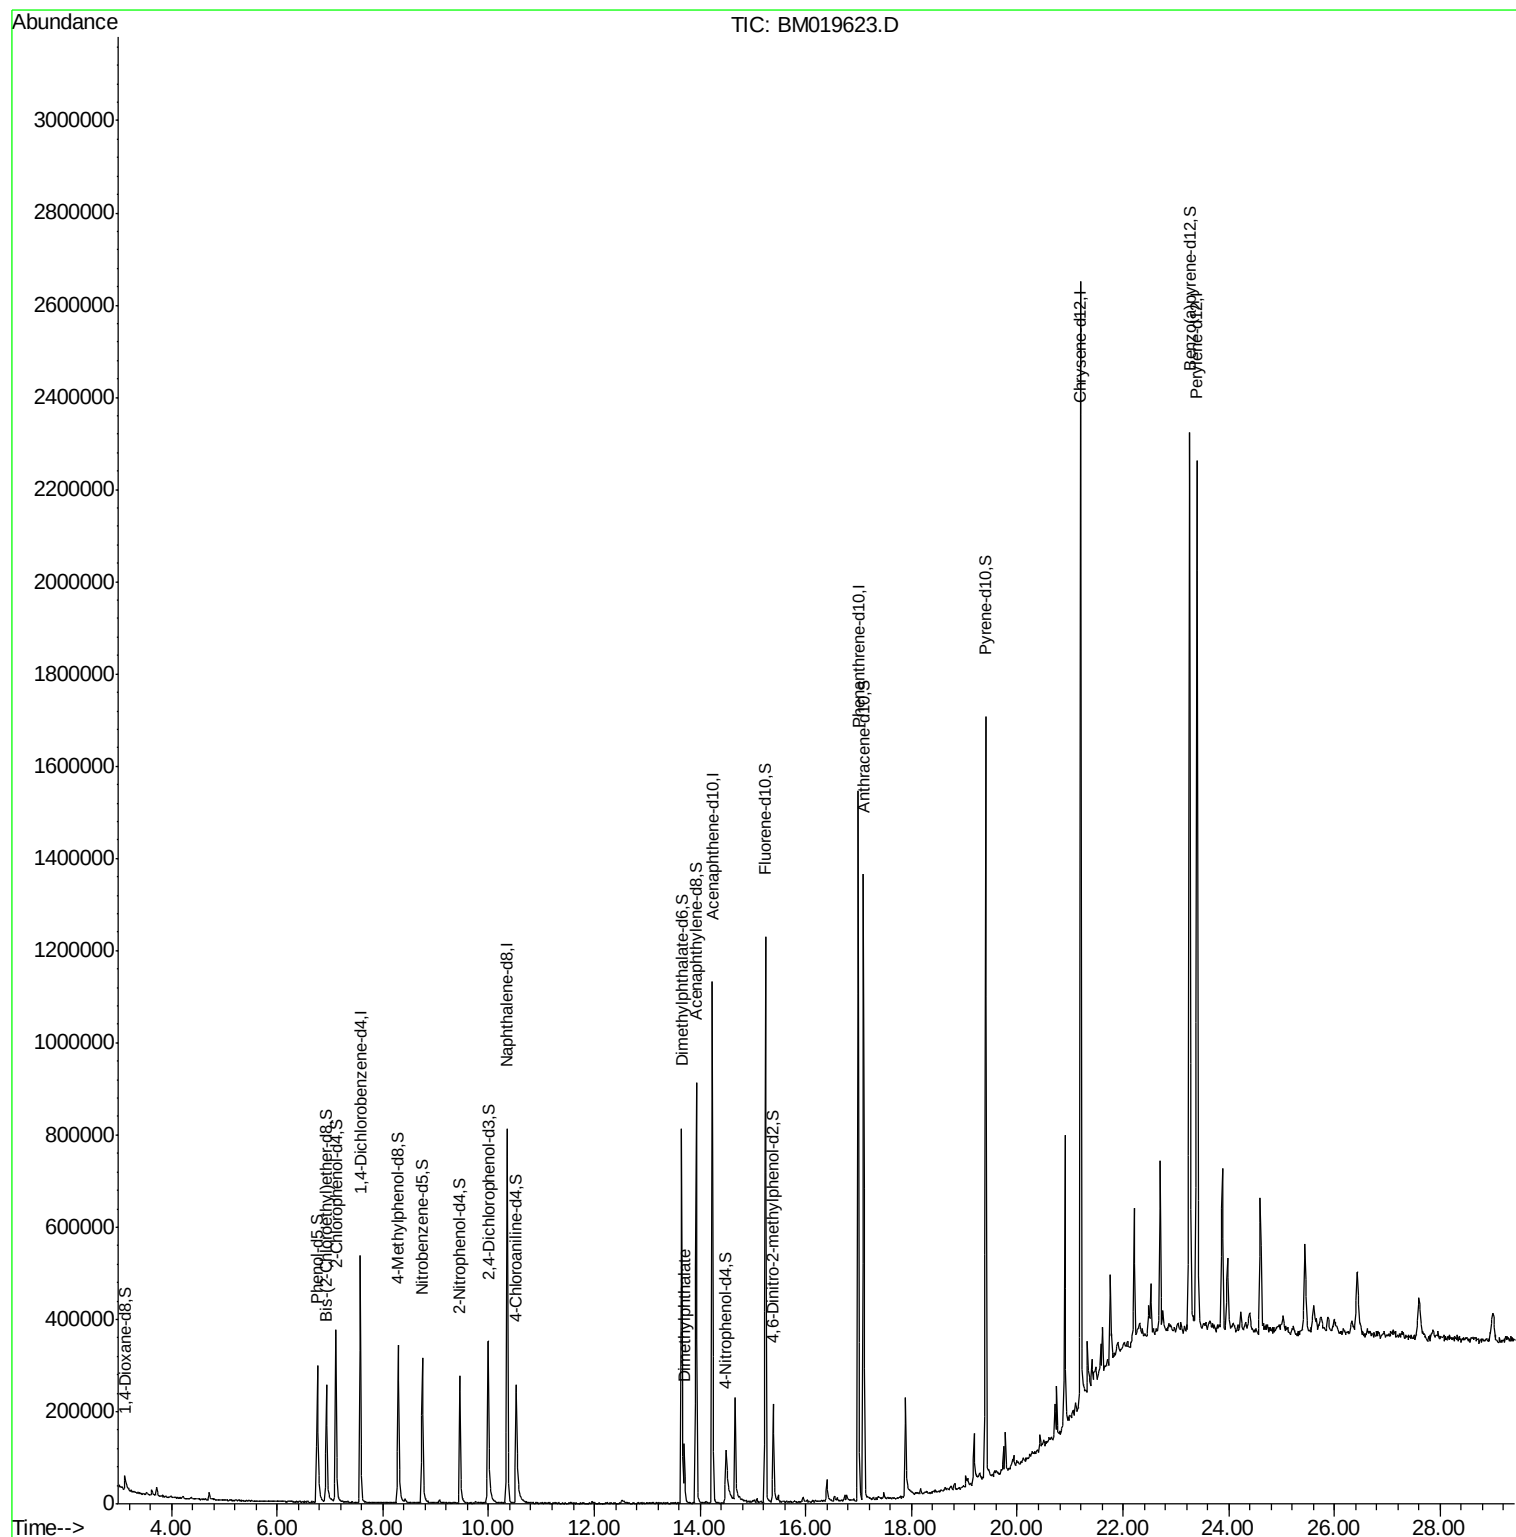

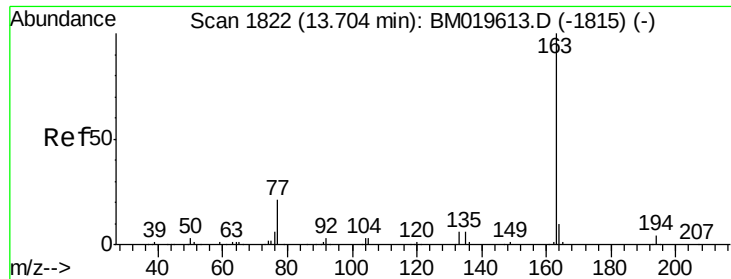

#45

Dimethylphthalate

Concen: 2.731 ng/ul

RT: 13.70 min Scan# 1822

Delta R.T. -0.01 min

Lab File: BM019623.D

Acq: 30 Mar 2019 17:26

Instrument :

BNA_M

ClientSampleId :

BF5L3


Tgt Ion:163 Resp: 78566

Ion Ratio Lower Upper

163 100

194 4.0 4.0 6.0#

164 9.1 8.4 12.6

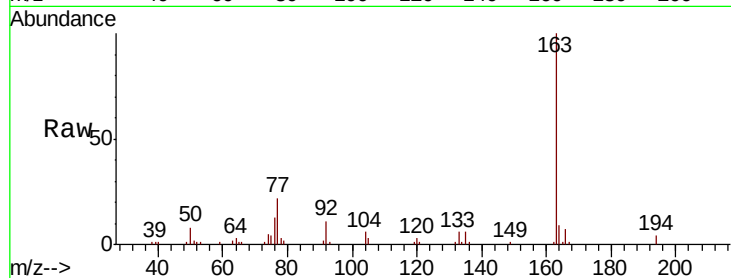

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

