

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM033019\
 Data File : BM019636.D
 Acq On : 31 Mar 2019 01:20
 Operator : JU/SJ
 Sample : K2068-12
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF5K8

Quant Time: Mar 31 02:11:47 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 29 14:33:17 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	152420	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	688902	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.23	164	388451	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.99	188	892615	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	1117909	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	1310813	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.12	96	19683	5.06	ng/uL	0.00
5) Phenol-d5	6.76	99	210661	15.52	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	139721	15.38	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	171841	16.70	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	175790	17.25	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	76827	15.63	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	87782	16.05	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	154828	15.00	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	227551	18.36	ng/ul	0.00
44) Dimethylphthalate-d6	13.65	166	534067	17.04	ng/ul	-0.01
47) Acenaphthylene-d8	13.93	160	667952	17.04	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	58483	11.90	ng/ul	0.01
58) Fluorene-d10	15.23	176	471714	17.47	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	43136	7.31	ng/ul	0.00
71) Anthracene-d10	17.09	188	757669	17.69	ng/ul	0.00
79) Pyrene-d10	19.40	212	882063	17.08	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	1179988	16.98	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.70	163	77724	2.472	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM033019\
Data File : BM019636.D
Acq On : 31 Mar 2019 01:20
Operator : JU/SJ
Sample : K2068-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF5K8

Quant Time: Mar 31 02:11:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 29 14:33:17 2019
Response via : Initial Calibration

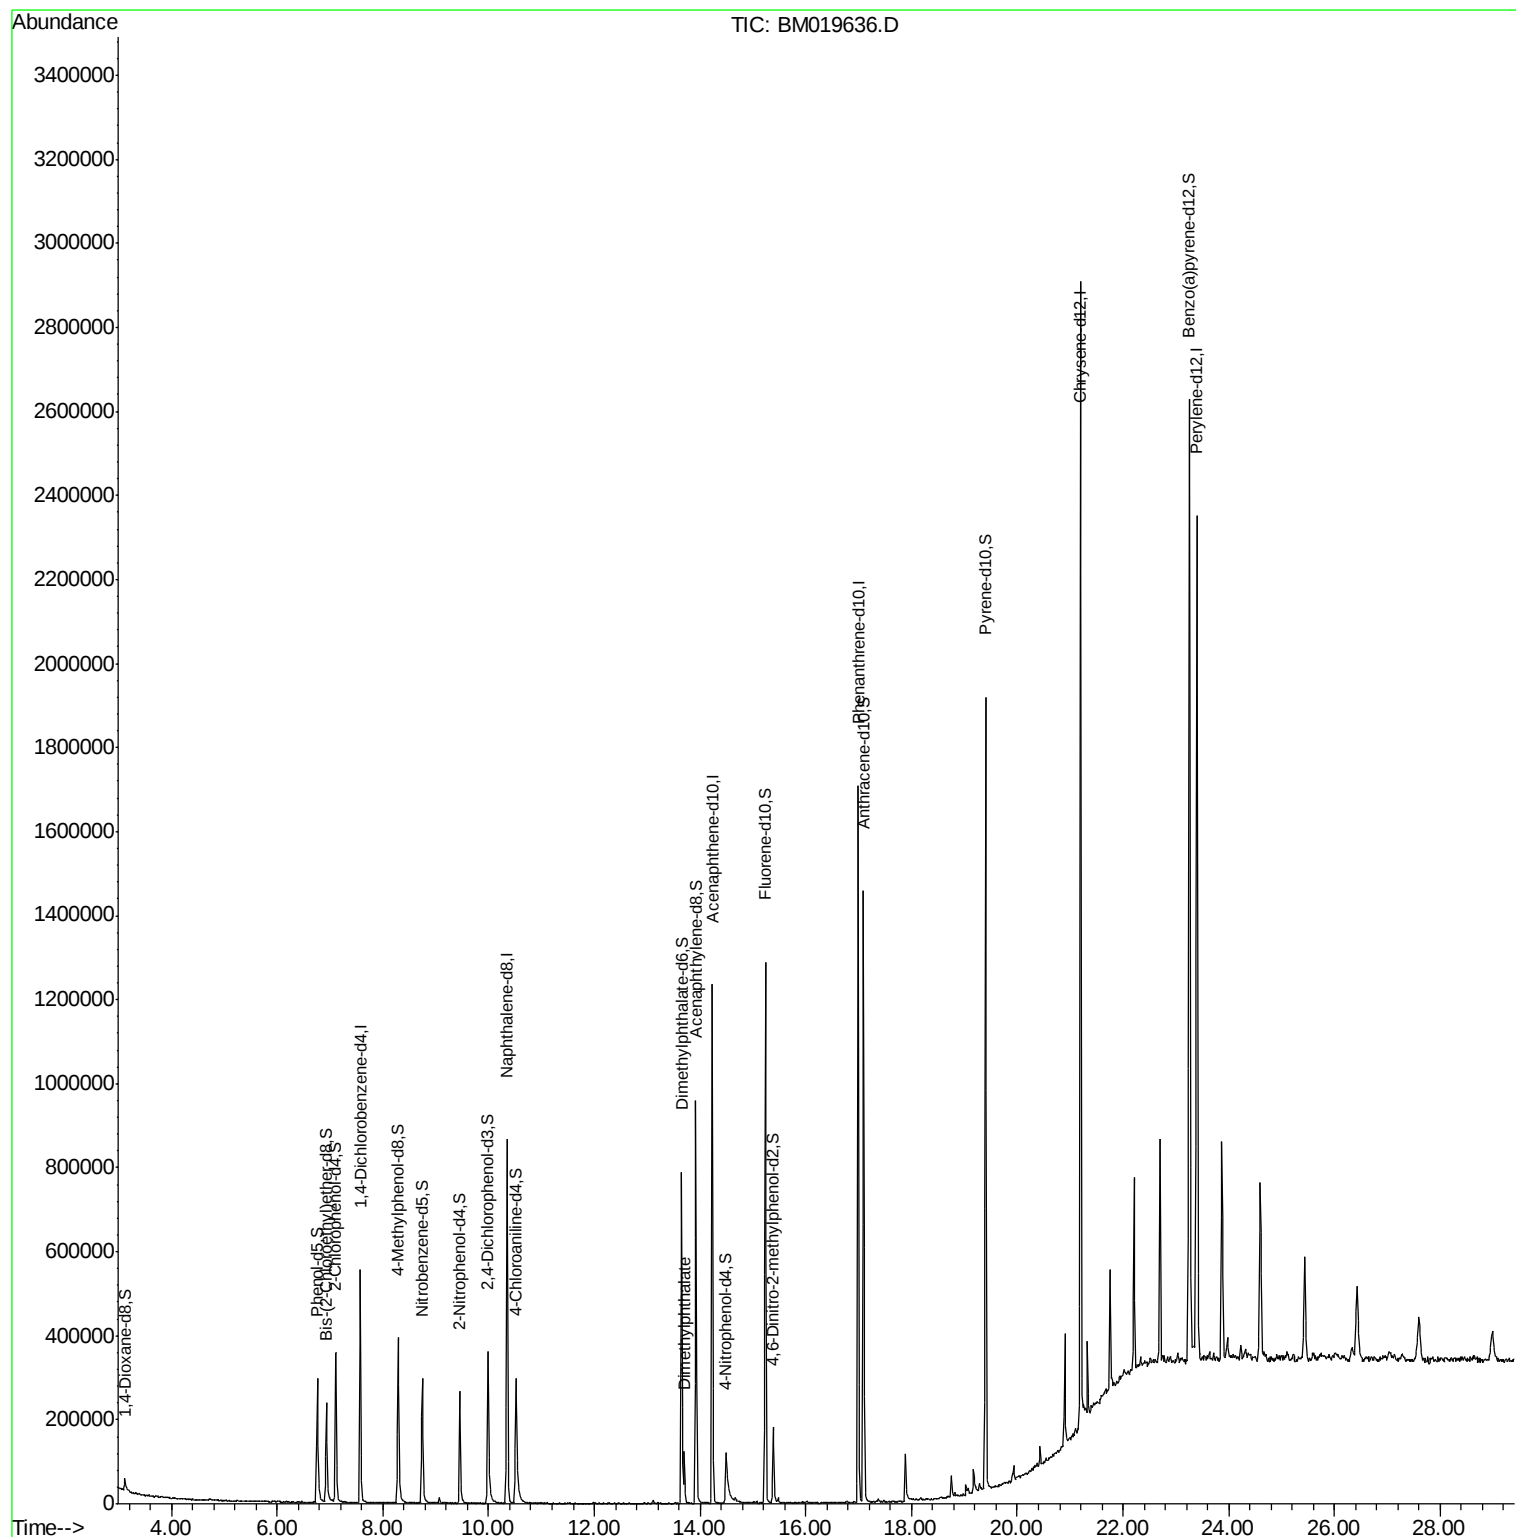

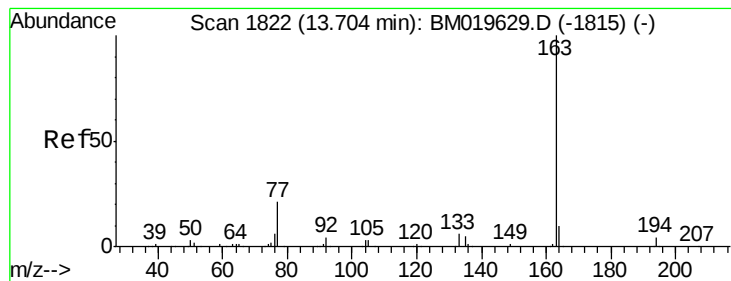

#45

Dimethylphthalate

Concen: 2.472 ng/ul

RT: 13.70 min Scan# 1822

Delta R.T. -0.01 min

Lab File: BM019636.D

Acq: 31 Mar 2019 01:20

Instrument :

BNA_M

ClientSampleId :

BF5K8


Tgt Ion:163 Resp: 77724

Ion Ratio Lower Upper

163 100

194 4.9 4.0 6.0

164 9.3 8.4 12.6

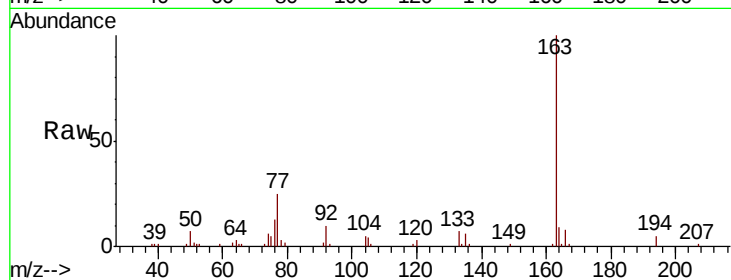

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

