

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM033019\
 Data File : BM019639.D
 Acq On : 31 Mar 2019 03:09
 Operator : JU/SJ
 Sample : K2068-17
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF5L1

Manual Integrations
 APPROVED

Sohil
 4/1/2019 5:50:58 PM

Quant Time: Mar 31 04:00:49 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Mar 31 02:55:53 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	158547	20.00	ng/ul	0.00
18) Naphthalene-d8	10.35	136	699951	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.23	164	390822	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.99	188	893317	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	1121830	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	1279704	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.12	96	17196	4.25	ng/uL	0.00
5) Phenol-d5	6.76	99	180143	12.76	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	127458	13.48	ng/ul	0.00
9) 2-Chlorophenol-d4	7.11	132	147864	13.82	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	147253	13.89	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	68439	13.71	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	76035	13.68	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	130682	12.46	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	182969	14.53	ng/ul	0.00
44) Dimethylphthalate-d6	13.66	166	468089	14.84	ng/ul	0.00
47) Acenaphthylene-d8	13.93	160	532285	13.50	ng/ul	0.00
52) 4-Nitrophenol-d4	14.50	143	46419m	9.39	ng/ul	0.02
58) Fluorene-d10	15.23	176	391856	14.42	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	39762	6.73	ng/ul	0.00
71) Anthracene-d10	17.09	188	603658	14.08	ng/ul	0.00
79) Pyrene-d10	19.40	212	684209	13.20	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	871595	12.85	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.70	163	79796	2.522	ng/ul#	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM033019\
Data File : BM019639.D
Acq On : 31 Mar 2019 03:09
Operator : JU/SJ
Sample : K2068-17
Misc :
ALS Vial : 27 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BF5L1

Manual Integrations
APPROVED

Sohil
4/1/2019 5:50:58 PM

Quant Time: Mar 31 04:00:49 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Mar 31 02:55:53 2019
Response via : Initial Calibration

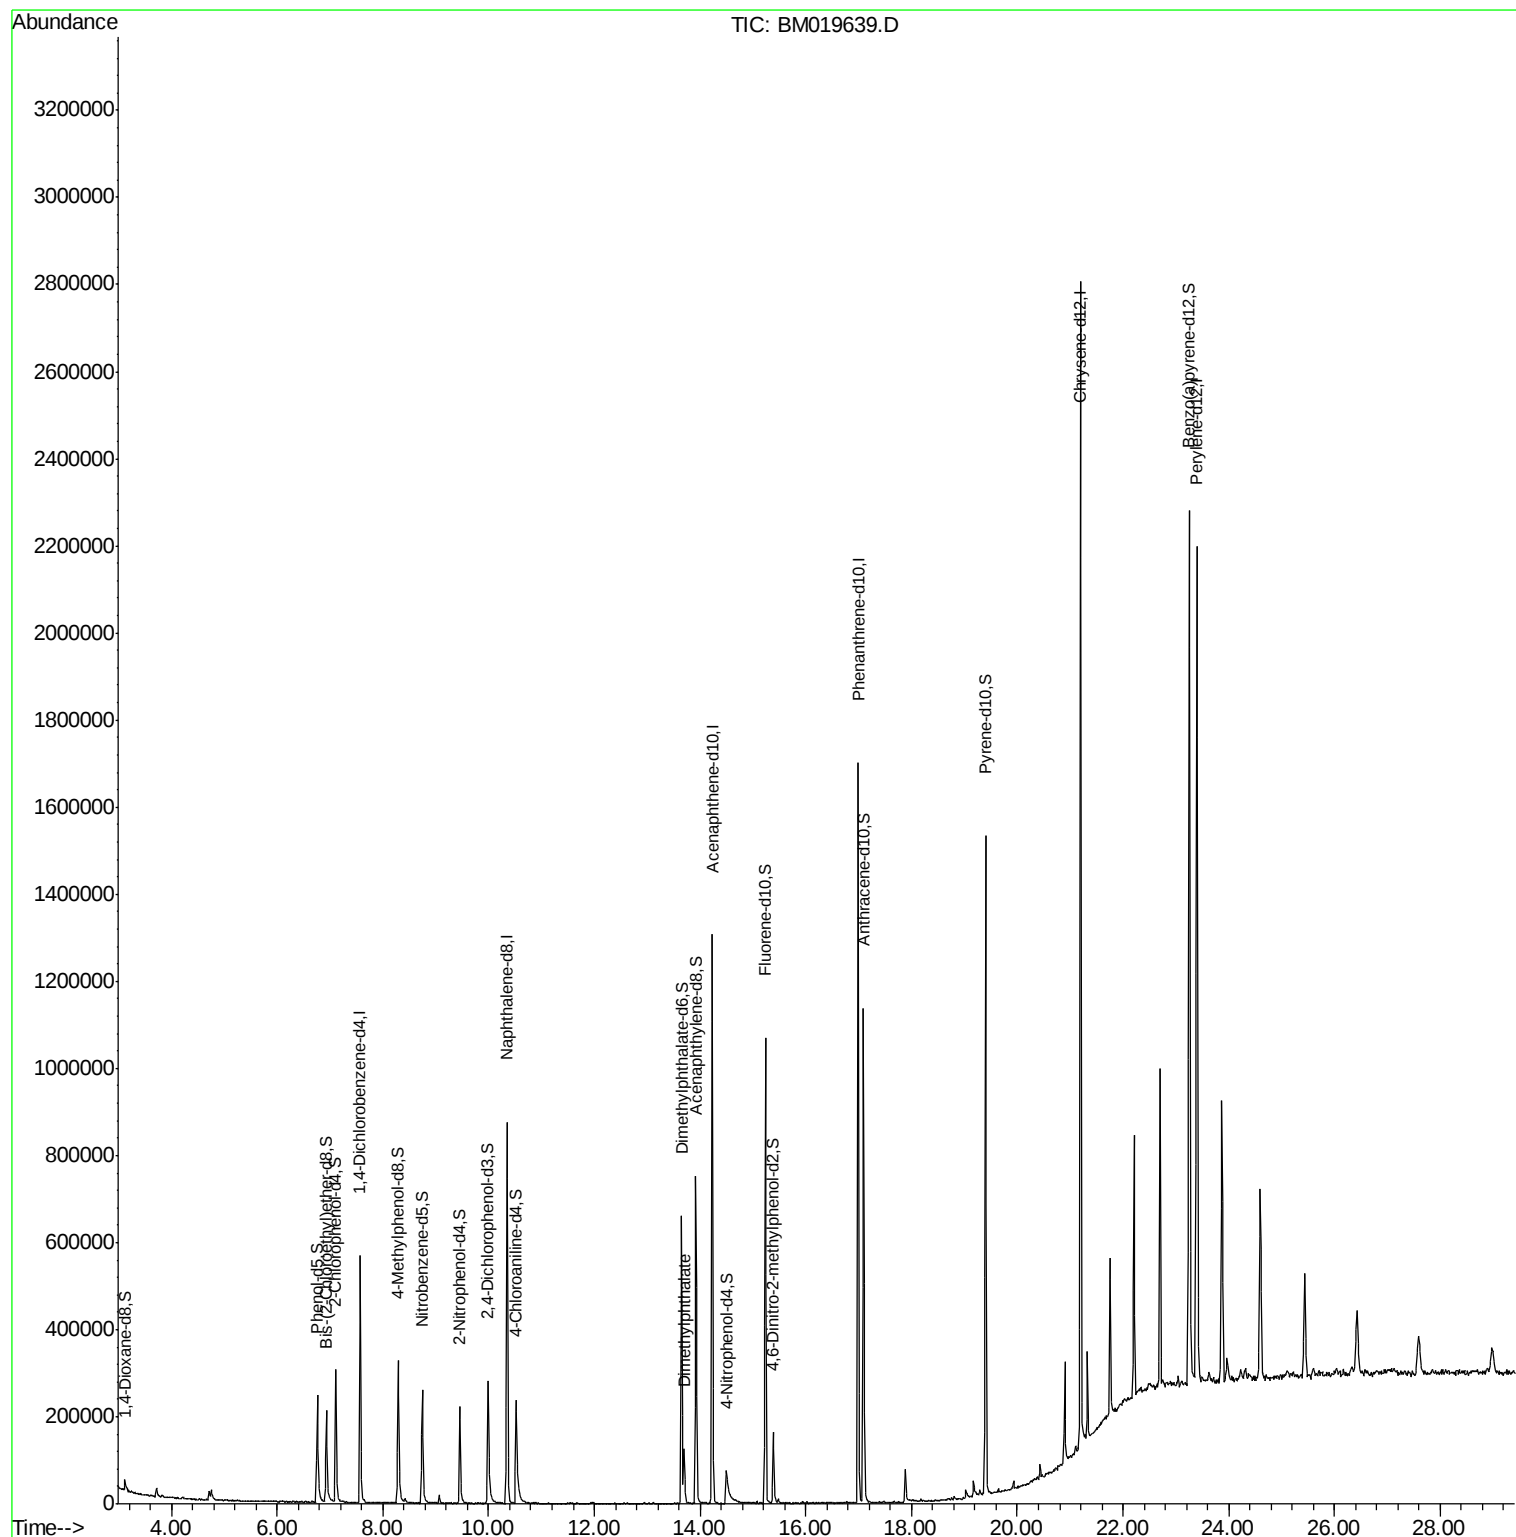

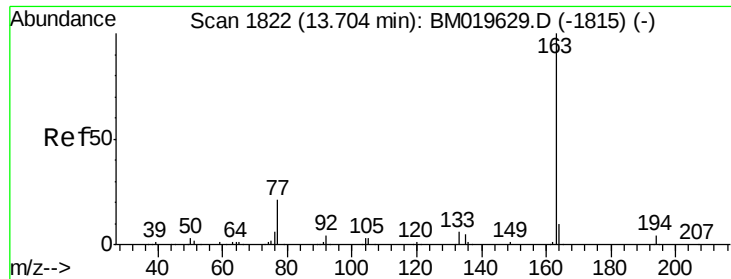


#45
 Dimethylphthalate
 Concen: 2.522 ng/ul
 RT: 13.70 min Scan# 1822
 Delta R.T. -0.01 min
 Lab File: BM019639.D
 Acq: 31 Mar 2019 03:09

Instrument :
 BNA_M
 ClientSampleId :
 BF5L1

Tgt Ion	Ratio	Resp Lower	Resp Upper
163	100		
194	3.6	4.0	6.0#
164	9.7	8.4	12.6

Manual Integrations
 APPROVED

Sohil
 4/1/2019 5:50:58 PM

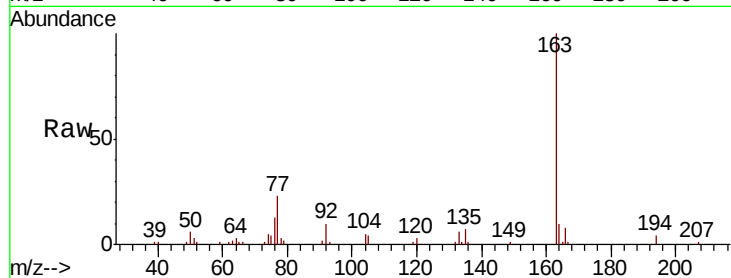

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

