

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM033019\
 Data File : BM019643.D
 Acq On : 31 Mar 2019 05:35
 Operator : JU/SJ
 Sample : K2068-24
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF5K5

Quant Time: Apr 01 01:17:03 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 29 14:33:17 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	141225	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.35	136	632200	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.23	164	352229	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.99	188	811516	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	1051005	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	1242419	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.12	96	18644	5.17	ng/uL	0.00
5) Phenol-d5	6.76	99	237642	18.90	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	167325	19.87	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	195960	20.56	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	192557	20.40	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	92173	20.44	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	104041	20.73	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	172072	18.17	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	240768	21.17	ng/ul	0.00
44) Dimethylphthalate-d6	13.65	166	612207	21.54	ng/ul	-0.01
47) Acenaphthylene-d8	13.92	160	707312	19.90	ng/ul	-0.01
52) 4-Nitrophenol-d4	14.49	143	69125	15.52	ng/ul	0.01
58) Fluorene-d10	15.23	176	517101	21.12	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	59685	11.12	ng/ul	0.00
71) Anthracene-d10	17.09	188	838564	21.53	ng/ul	0.00
79) Pyrene-d10	19.40	212	975280	20.09	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	1282129	19.47	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.70	163	67962	2.383	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM033019\
Data File : BM019643.D
Acq On : 31 Mar 2019 05:35
Operator : JU/SJ
Sample : K2068-24
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF5K5

Quant Time: Apr 01 01:17:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 29 14:33:17 2019
Response via : Initial Calibration

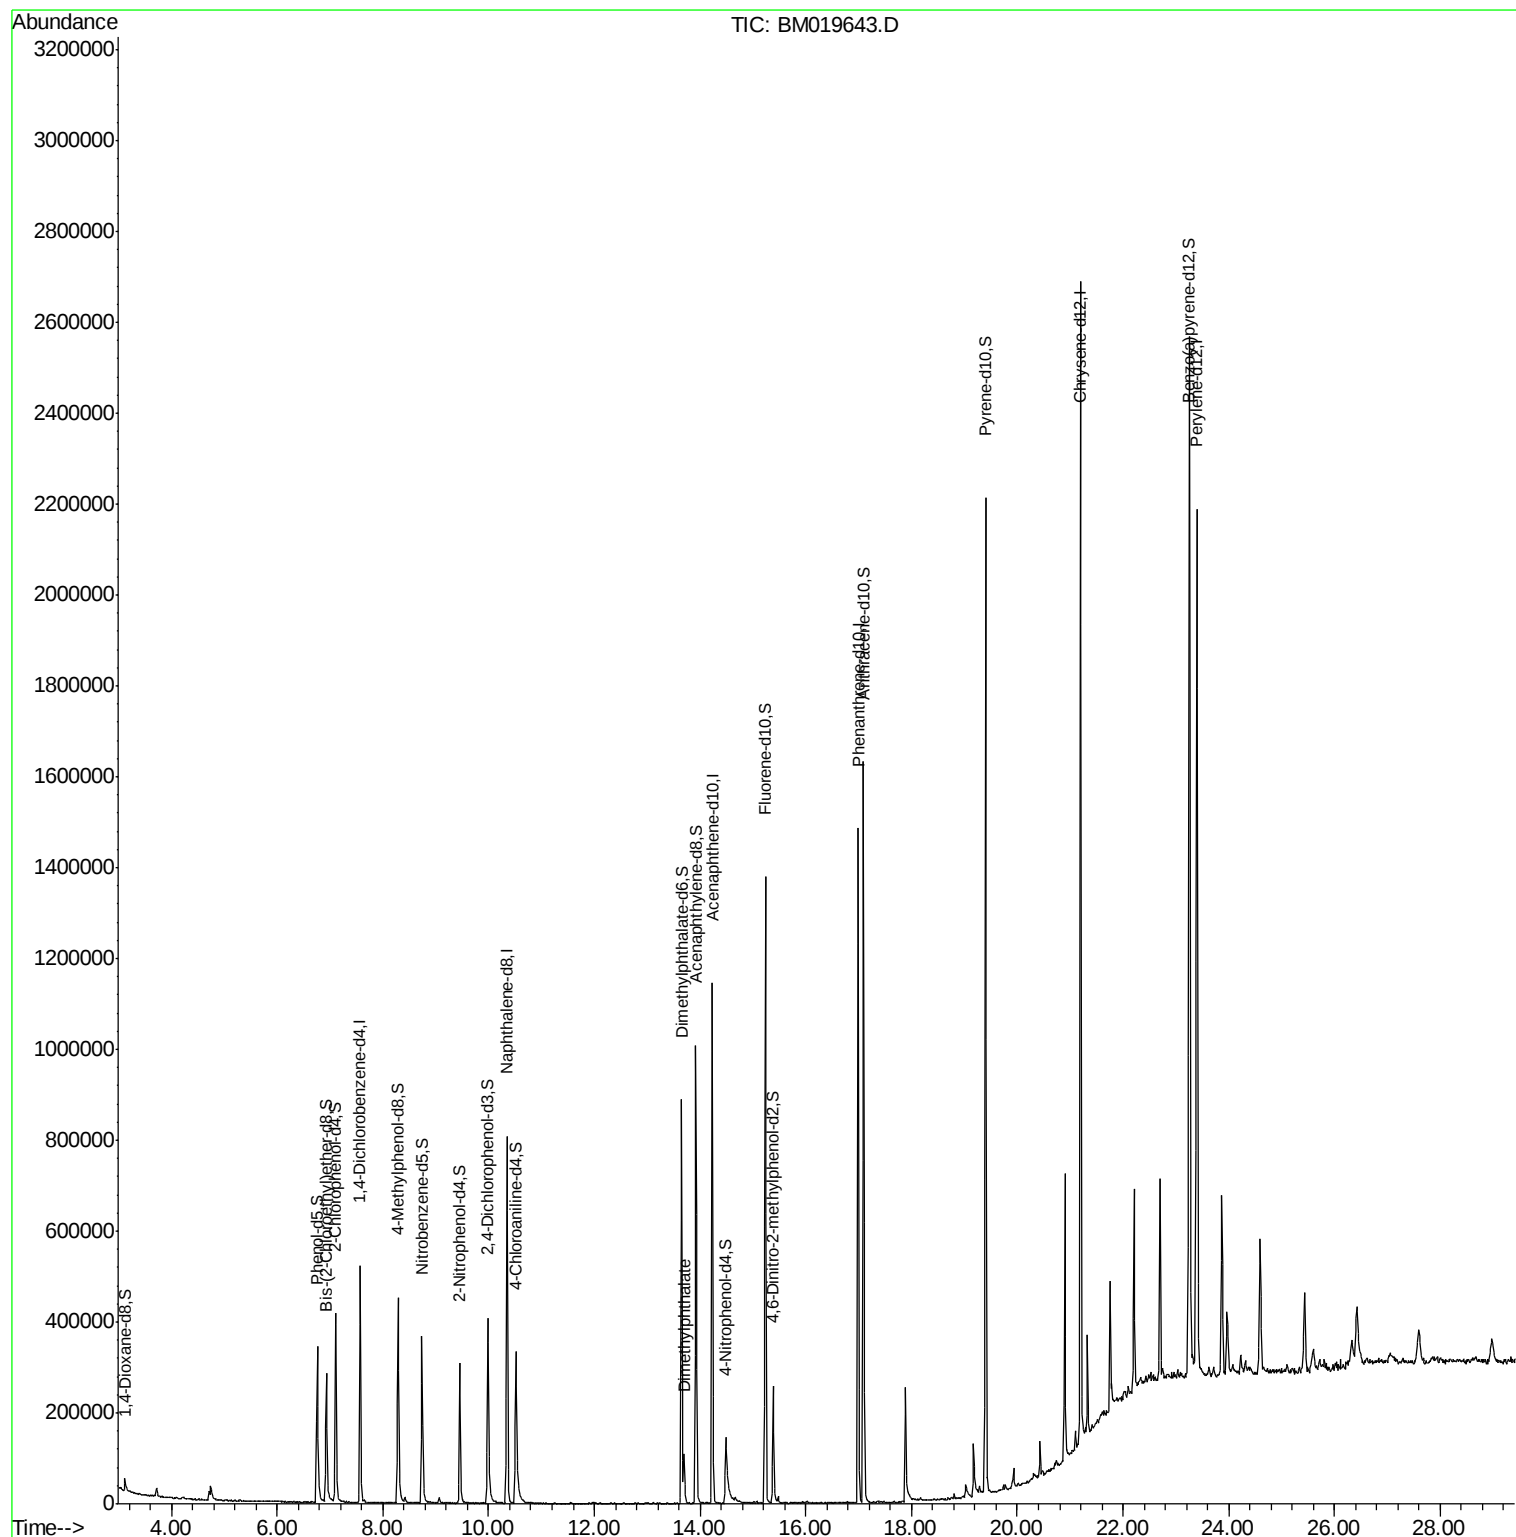

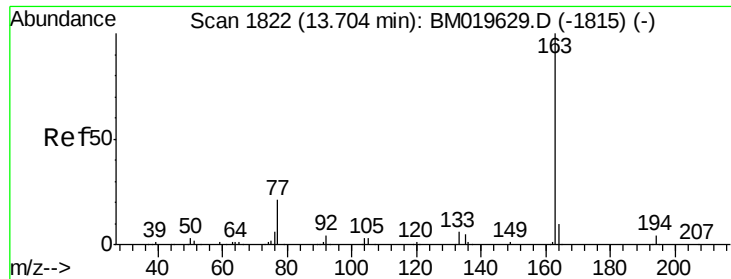

#45

Dimethylphthalate

Concen: 2.383 ng/ul

RT: 13.70 min Scan# 1822

Delta R.T. -0.01 min

Lab File: BM019643.D

Acq: 31 Mar 2019 05:35

Instrument :

BNA_M

ClientSampleId :

BF5K5


Tgt Ion:163 Resp: 67962

Ion Ratio Lower Upper

163 100

194 4.1 4.0 6.0

164 11.1 8.4 12.6

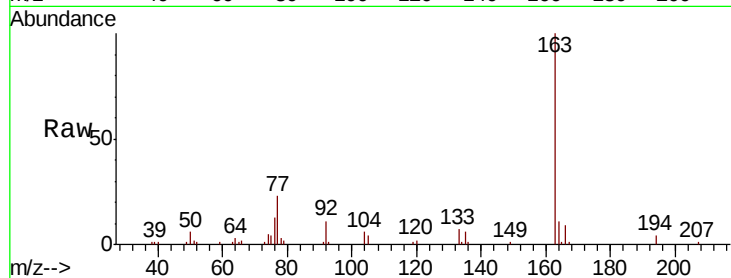

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

