

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_M\DATA\BM040119\  
 Data File : BM019655.D  
 Acq On : 01 Apr 2019 15:10  
 Operator : JU/SJ  
 Sample : K2119-03  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 BF5A0

Quant Time: Apr 02 04:00:16 2019  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM032219MA.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue Apr 02 03:56:34 2019  
 Response via : Initial Calibration

| Internal Standards        | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|---------------------------|-------|------|----------|-------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4 | 7.57  | 152  | 109026   | 20.00 | ng/ul | -0.01    |
| 18) Naphthalene-d8        | 10.35 | 136  | 493726   | 20.00 | ng/ul | 0.00     |
| 36) Acenaphthene-d10      | 14.23 | 164  | 285819   | 20.00 | ng/ul | -0.01    |
| 62) Phenanthrene-d10      | 16.99 | 188  | 675046   | 20.00 | ng/ul | 0.00     |
| 78) Chrysene-d12          | 21.20 | 240  | 884943   | 20.00 | ng/ul | 0.00     |
| 86) Perylene-d12          | 23.40 | 264  | 1021421  | 20.00 | ng/ul | -0.01    |

| System Monitoring Compounds    | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|--------------------------------|-------|------|----------|-------|-------|----------|
| 3) 1,4-Dioxane-d8              | 3.12  | 96   | 13056    | 4.69  | ng/uL | 0.00     |
| 5) Phenol-d5                   | 6.76  | 99   | 137604   | 14.17 | ng/ul | 0.00     |
| 7) Bis-(2-Chloroethyl)ether-d  | 6.93  | 67   | 92333    | 14.21 | ng/ul | 0.00     |
| 9) 2-Chlorophenol-d4           | 7.10  | 132  | 115347   | 15.68 | ng/ul | 0.00     |
| 13) 4-Methylphenol-d8          | 8.29  | 113  | 113716   | 15.60 | ng/ul | 0.00     |
| 19) Nitrobenzene-d5            | 8.75  | 128  | 52653    | 14.95 | ng/ul | 0.00     |
| 22) 2-Nitrophenol-d4           | 9.46  | 143  | 58881    | 15.02 | ng/ul | 0.00     |
| 26) 2,4-Dichlorophenol-d3      | 9.99  | 165  | 96344    | 13.03 | ng/ul | 0.00     |
| 29) 4-Chloroaniline-d4         | 10.52 | 131  | 140058   | 15.77 | ng/ul | 0.00     |
| 44) Dimethylphthalate-d6       | 13.65 | 166  | 361335   | 15.67 | ng/ul | -0.01    |
| 47) Acenaphthylene-d8          | 13.92 | 160  | 419939   | 14.56 | ng/ul | -0.01    |
| 52) 4-Nitrophenol-d4           | 14.50 | 143  | 34141    | 9.44  | ng/ul | 0.02     |
| 58) Fluorene-d10               | 15.23 | 176  | 313959   | 15.80 | ng/ul | 0.00     |
| 63) 4,6-Dinitro-2-methylphenol | 15.39 | 200  | 34371    | 7.70  | ng/ul | 0.00     |
| 71) Anthracene-d10             | 17.09 | 188  | 500883   | 15.46 | ng/ul | 0.00     |
| 79) Pyrene-d10                 | 19.40 | 212  | 599738   | 14.67 | ng/ul | 0.00     |
| 90) Benzo(a)pyrene-d12         | 23.26 | 264  | 770984   | 14.24 | ng/ul | -0.01    |


| Target Compounds      | R.T.  | QIon | Response | Conc  | Units  | Qvalue |
|-----------------------|-------|------|----------|-------|--------|--------|
| 45) Dimethylphthalate | 13.70 | 163  | 92176    | 3.984 | ng/ul# | 98     |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA\_M\DATA\BM040119\  
Data File : BM019655.D  
Acq On : 01 Apr 2019 15:10  
Operator : JU/SJ  
Sample : K2119-03  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
BF5A0

Quant Time: Apr 02 04:00:16 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM032219MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Tue Apr 02 03:56:34 2019  
Response via : Initial Calibration

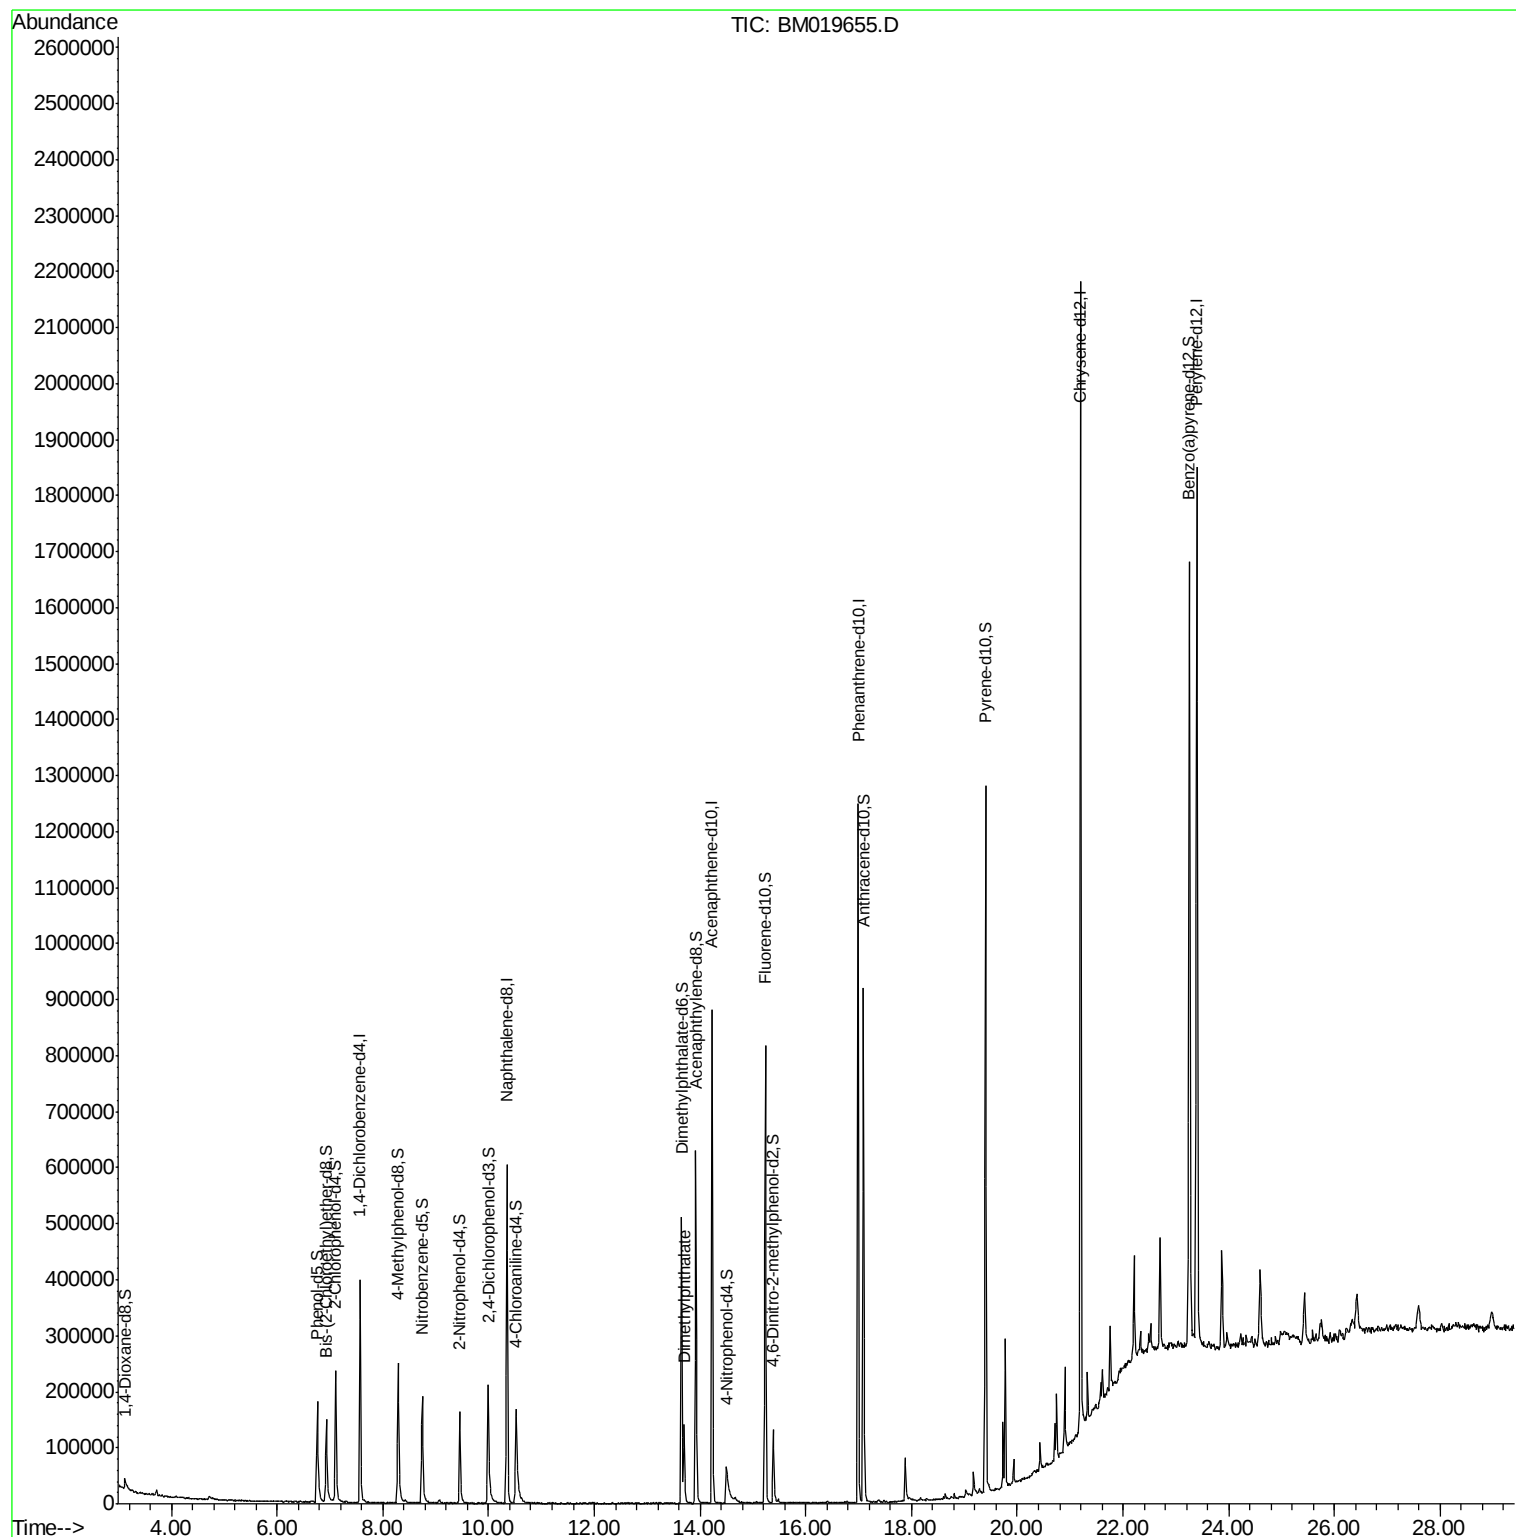

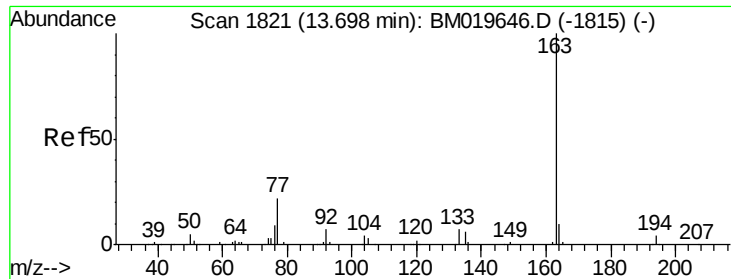

#45

Dimethylphthalate

Concen: 3.984 ng/ul

RT: 13.70 min Scan# 1821

Delta R.T. -0.01 min

Lab File: BM019655.D

Acq: 01 Apr 2019 15:10

Instrument :

BNA\_M

ClientSampleId :

BF5A0


Tgt Ion:163 Resp: 92176

Ion Ratio Lower Upper

163 100

194 3.8 4.0 6.0#

164 10.0 8.4 12.6

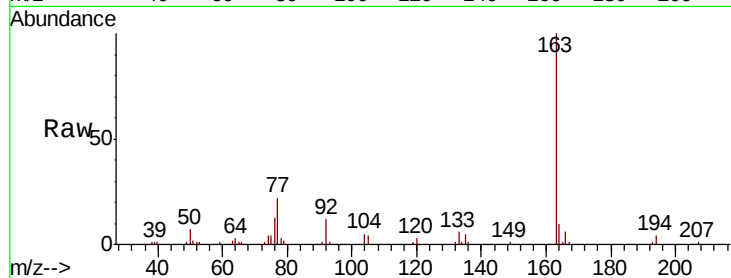

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

