

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040119\
 Data File : BM019657.D
 Acq On : 01 Apr 2019 16:22
 Operator : JU/SJ
 Sample : K2119-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF5A2

Quant Time: Apr 02 04:00:26 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 02 03:56:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	131249	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.35	136	565766	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.23	164	325572	20.00	ng/ul	-0.01
62) Phenanthrene-d10	16.99	188	730614	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	856723	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	949443	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.12	96	18341	5.47	ng/uL	0.00
5) Phenol-d5	6.76	99	154894	13.25	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	106293	13.58	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	132152	14.92	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	133198	15.18	ng/ul	0.00
19) Nitrobenzene-d5	8.74	128	59910	14.84	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.50	143	2322	0.52	ng/ul	0.04
26) 2,4-Dichlorophenol-d3	9.99	165	110411	13.03	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	156521	15.38	ng/ul	0.00
44) Dimethylphthalate-d6	13.65	166	419760	15.98	ng/ul	-0.01
47) Acenaphthylene-d8	13.92	160	473650	14.42	ng/ul	-0.01
52) 4-Nitrophenol-d4	14.50	143	37350	9.07	ng/ul	0.02
58) Fluorene-d10	15.23	176	343536	15.18	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	41969	8.69	ng/ul	0.00
71) Anthracene-d10	17.09	188	537752	15.34	ng/ul	-0.01
79) Pyrene-d10	19.40	212	628154	15.87	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	727280	14.45	ng/ul	0.00


Target Compounds					Qvalue	
45) Dimethylphthalate	13.70	163	94175	3.573	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040119\
Data File : BM019657.D
Acq On : 01 Apr 2019 16:22
Operator : JU/SJ
Sample : K2119-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF5A2

Quant Time: Apr 02 04:00:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 02 03:56:34 2019
Response via : Initial Calibration

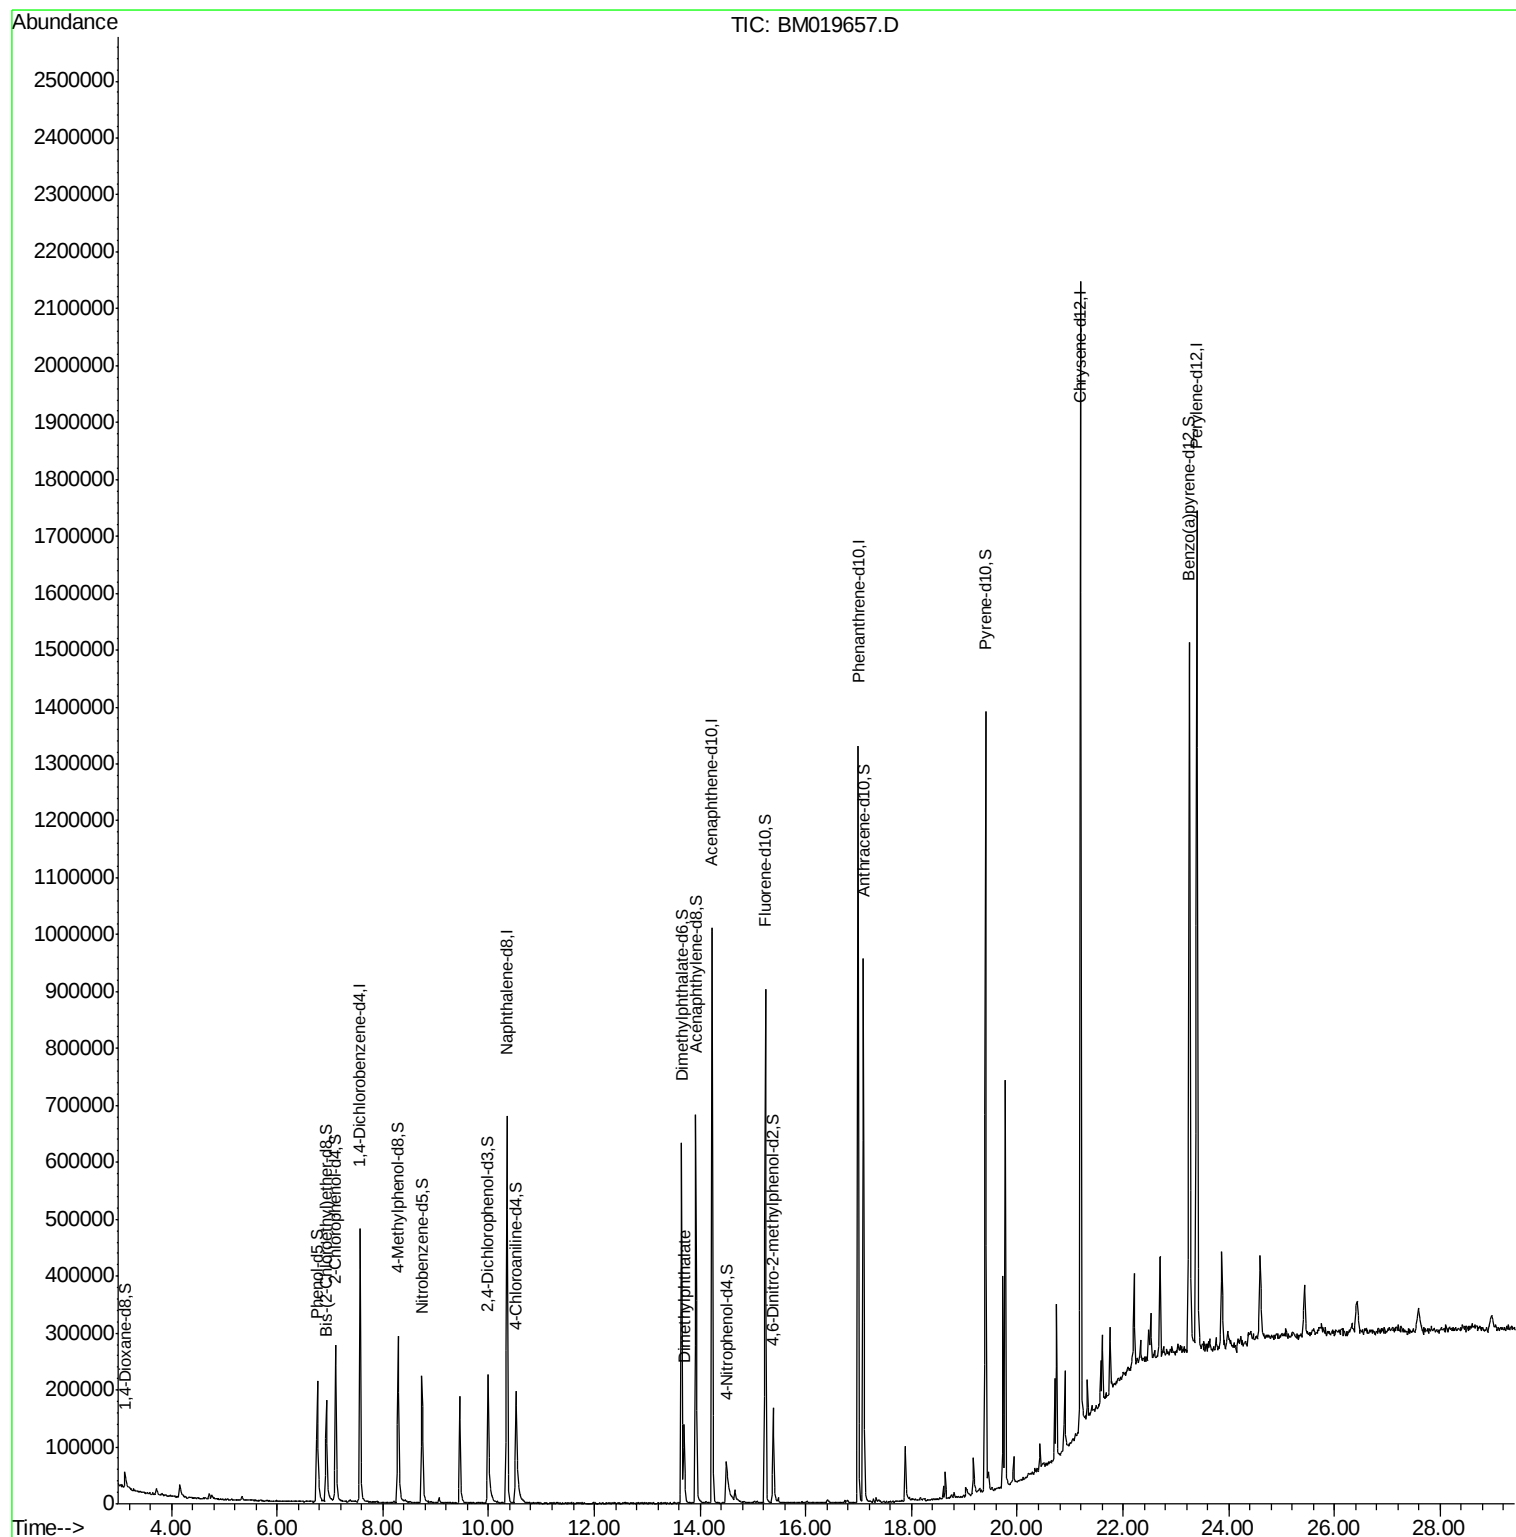

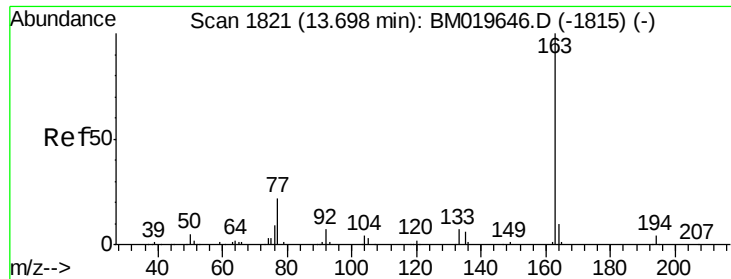

#45

Dimethylphthalate

Concen: 3.573 ng/ul

RT: 13.70 min Scan# 1822

Delta R.T. -0.01 min

Lab File: BM019657.D


Acq: 01 Apr 2019 16:22

Instrument :

BNA_M

ClientSampleId :

BF5A2

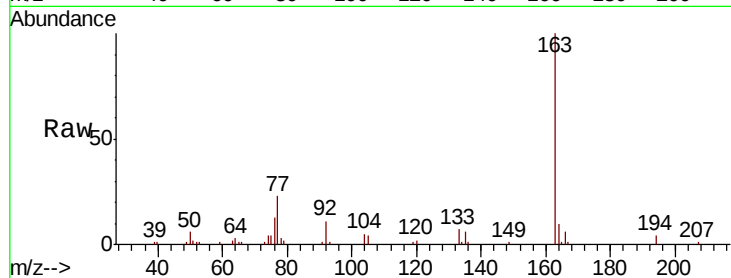


Tgt Ion:163 Resp: 94175

Ion Ratio Lower Upper

163 100

194 4.0 4.0 6.0

164 10.1 8.4 12.6

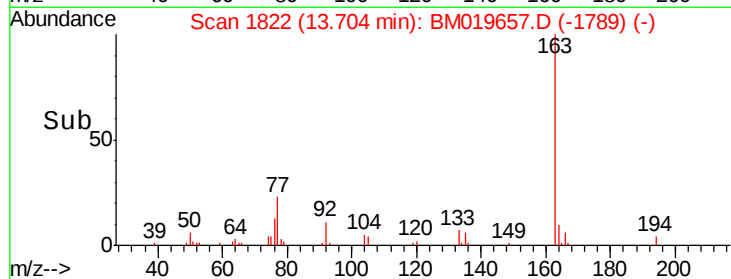

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

