

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040119\
 Data File : BM019671.D
 Acq On : 02 Apr 2019 00:46
 Operator : JU/SJ
 Sample : K2149-06
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF5H5

Quant Time: Apr 02 07:11:38 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 02 07:07:56 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	191401	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.35	136	857598	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.23	164	488031	20.00	ng/ul	-0.01
62) Phenanthrene-d10	16.99	188	1045980	20.00	ng/ul	-0.01
78) Chrysene-d12	21.20	240	880003	20.00	ng/ul	0.00
86) Perylene-d12	23.39	264	798875	20.00	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.12	96	21659	4.43	ng/uL	0.00
5) Phenol-d5	6.76	99	201141	11.80	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	145929	12.79	ng/ul	-0.01
9) 2-Chlorophenol-d4	7.10	132	164460	12.73	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	141138	11.03	ng/ul	0.00
19) Nitrobenzene-d5	8.74	128	79574	13.01	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.45	143	92380	13.57	ng/ul	-0.01
26) 2,4-Dichlorophenol-d3	9.98	165	153810	11.97	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.52	131	209297	13.57	ng/ul	0.00
44) Dimethylphthalate-d6	13.65	166	616057	15.64	ng/ul	-0.01
47) Acenaphthylene-d8	13.92	160	685971	13.93	ng/ul	-0.01
52) 4-Nitrophenol-d4	14.49	143	50622	8.20	ng/ul	0.01
58) Fluorene-d10	15.23	176	502704	14.82	ng/ul	-0.01
63) 4,6-Dinitro-2-methylphenol	15.38	200	68454	9.90	ng/ul	0.00
71) Anthracene-d10	17.09	188	772502	15.39	ng/ul	-0.01
79) Pyrene-d10	19.40	212	775977	19.09	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	591574	13.97	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.70	163	76053	1.925	ng/ul#	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040119\
Data File : BM019671.D
Acq On : 02 Apr 2019 00:46
Operator : JU/SJ
Sample : K2149-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF5H5

Quant Time: Apr 02 07:11:38 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 02 07:07:56 2019
Response via : Initial Calibration

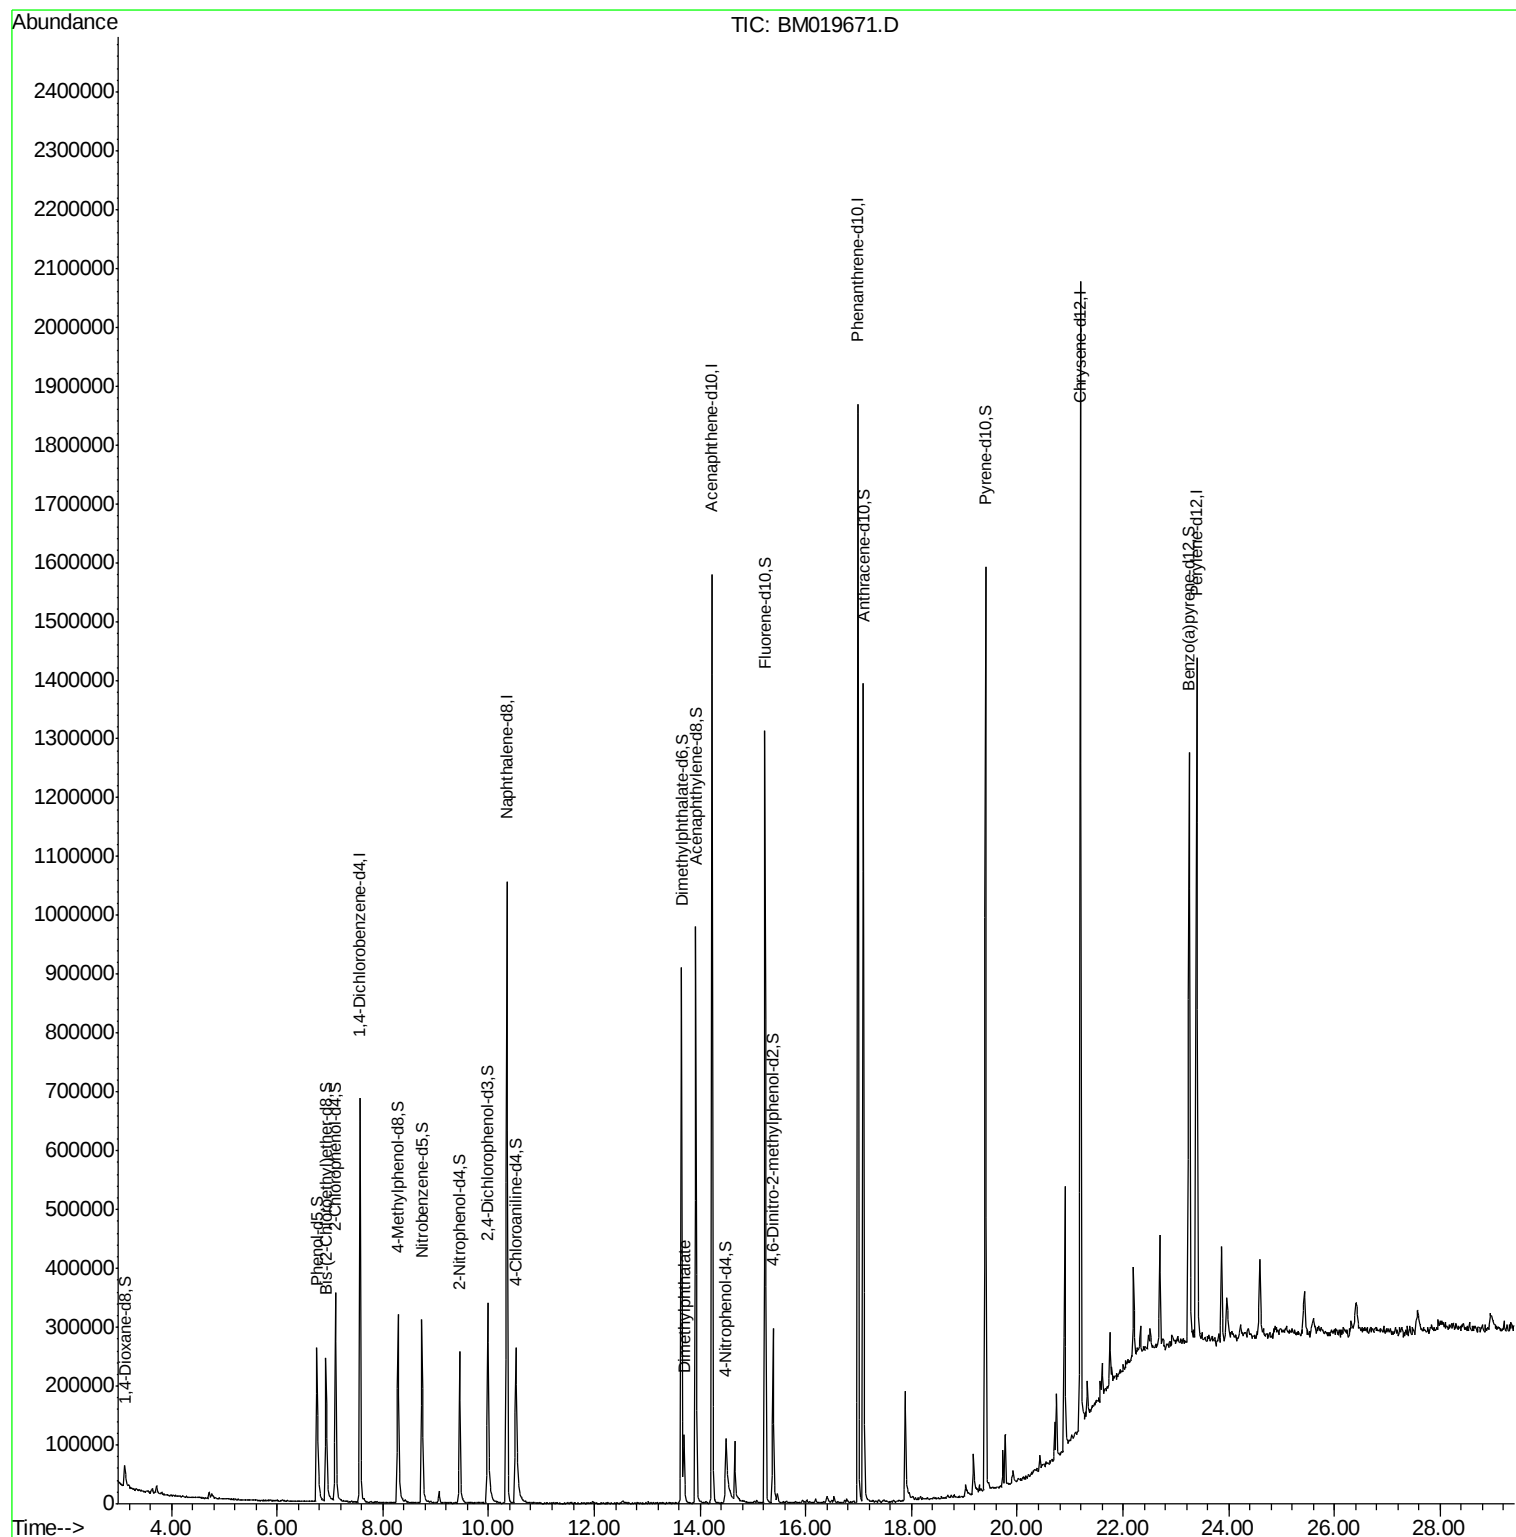

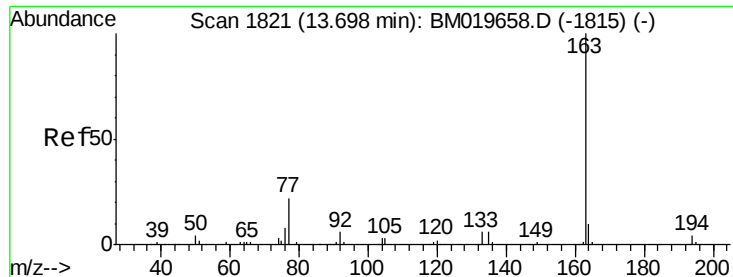

#45

Dimethylphthalate

Concen: 1.925 ng/ul

RT: 13.70 min Scan# 1821

Delta R.T. -0.01 min

Lab File: BM019671.D

Acq: 02 Apr 2019 00:46

Instrument :

BNA_M

ClientSampleId :

BF5H5


Tgt Ion:163 Resp: 76053

Ion Ratio Lower Upper

163 100

194 3.5 4.0 6.0#

164 11.2 8.4 12.6

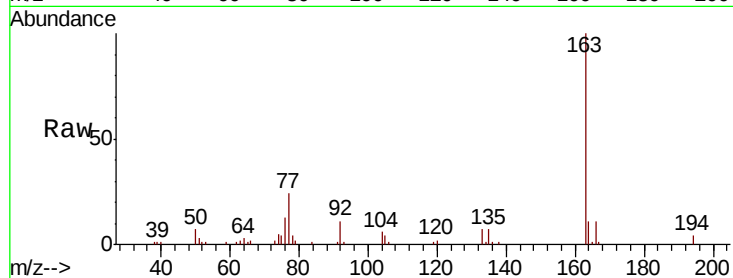

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

