


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040119\
Data File : BM019664.D
Acq On : 01 Apr 2019 20:34
Operator : JU/SJ
Sample : K2119-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF5A9

Manual Integrations
APPROVED

Sohil
4/2/2019 5:31:14 PM

Quant Time: Apr 02 07:46:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 02 07:07:56 2019
Response via : Initial Calibration

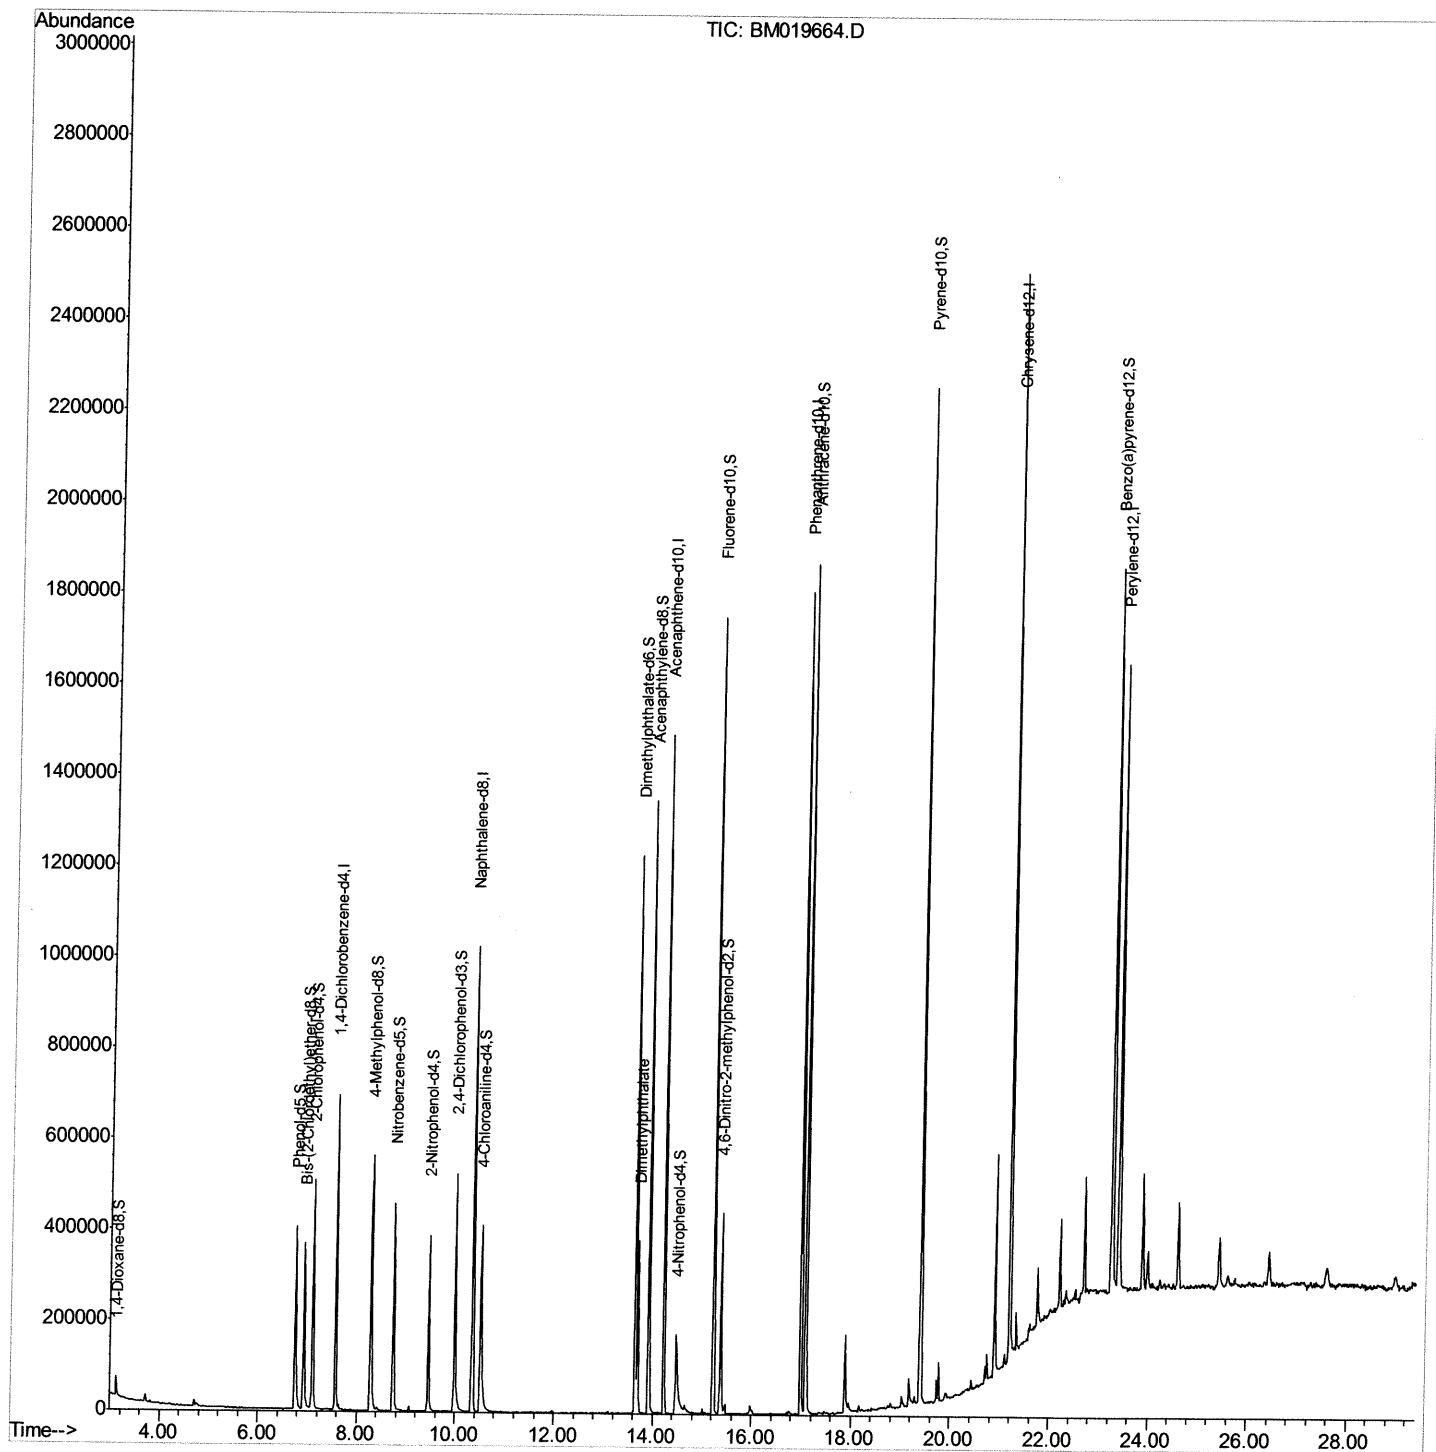

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040119\
Data File : BM019664.D
Acq On : 01 Apr 2019 20:34
Operator : JU/SJ
Sample : K2119-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
BF5A9

Manual Integrations
APPROVED

Sohil
4/2/2019 5:31:14 PM

Quant Time: Apr 02 07:11:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 02 07:07:56 2019
Response via : Initial Calibration

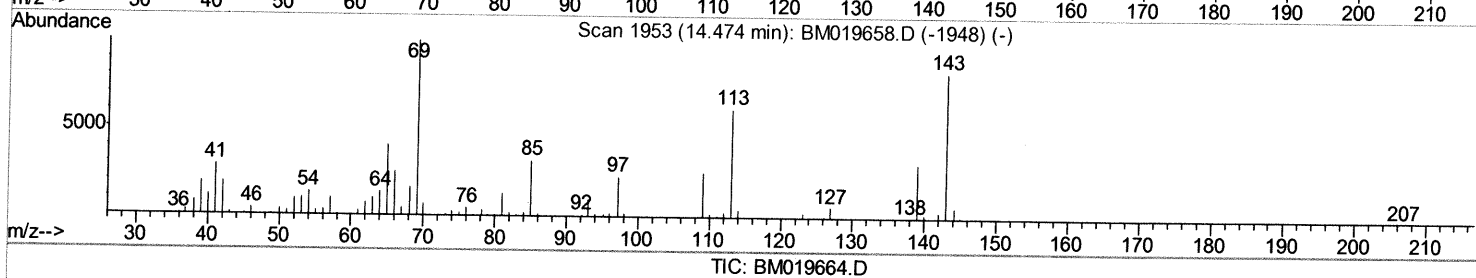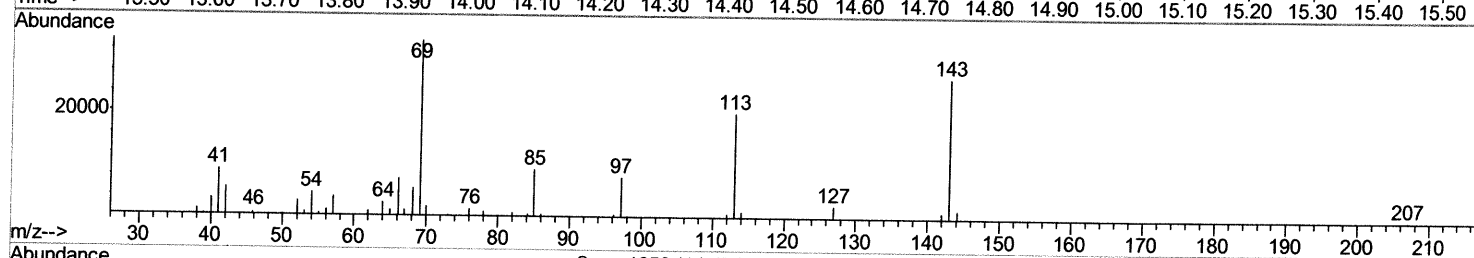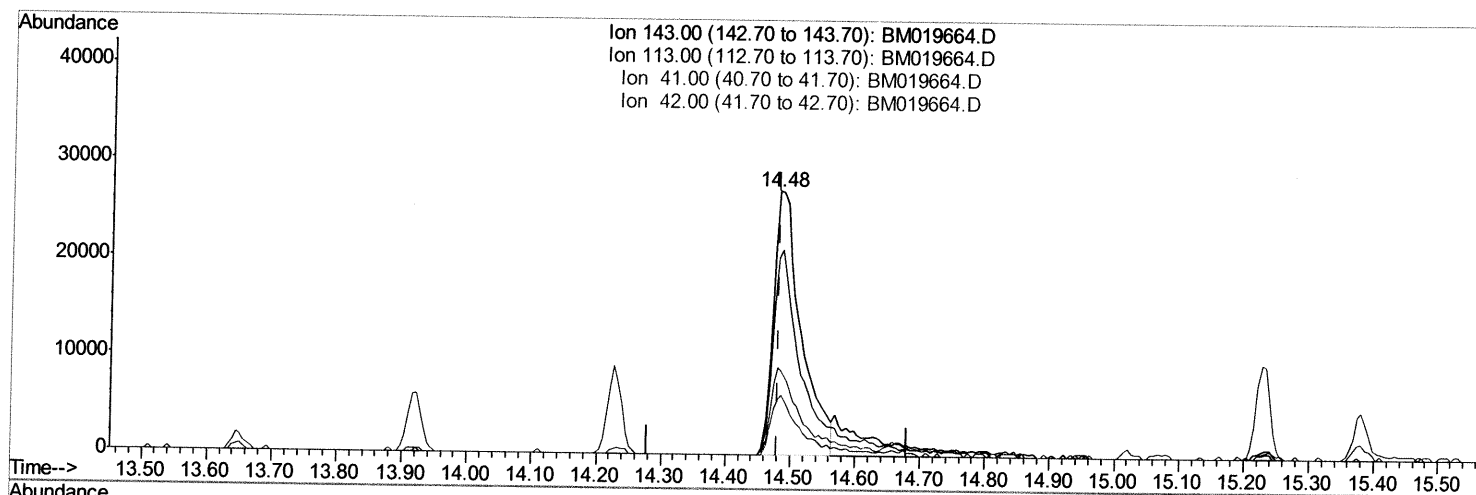

(52) 4-Nitrophenol-d4 (S)

14.480min (0.000) 13.47ng/ul

response 80595

Ion	Exp%	Act%
143.00	100	100
113.00	77.10	74.47
41.00	32.60	33.00
42.00	22.30	21.01

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040119\
 Data File : BM019664.D
 Acq On : 01 Apr 2019 20:34
 Operator : JU/SJ
 Sample : K2119-14
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF5A9

Manual Integrations
 APPROVED

Sohil
 4/2/2019 5:31:14 PM

Quant Time: Apr 02 07:11:07 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 02 07:07:56 2019
 Response via : Initial Calibration

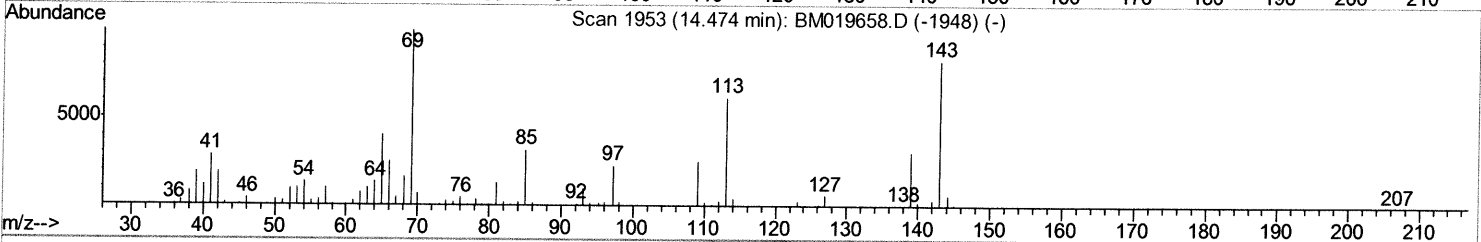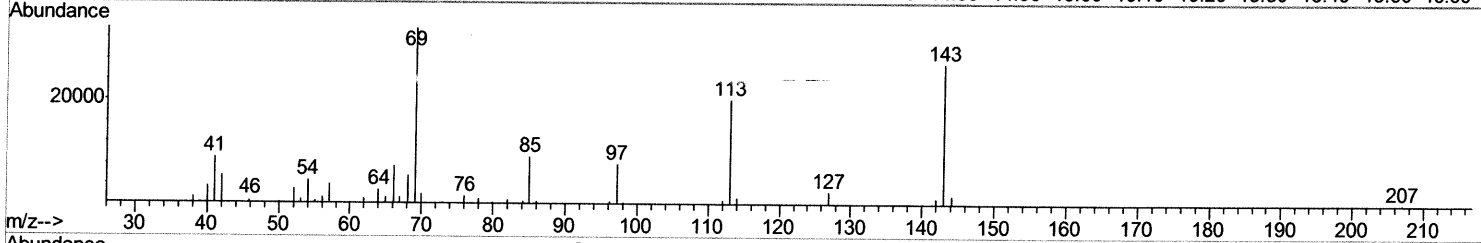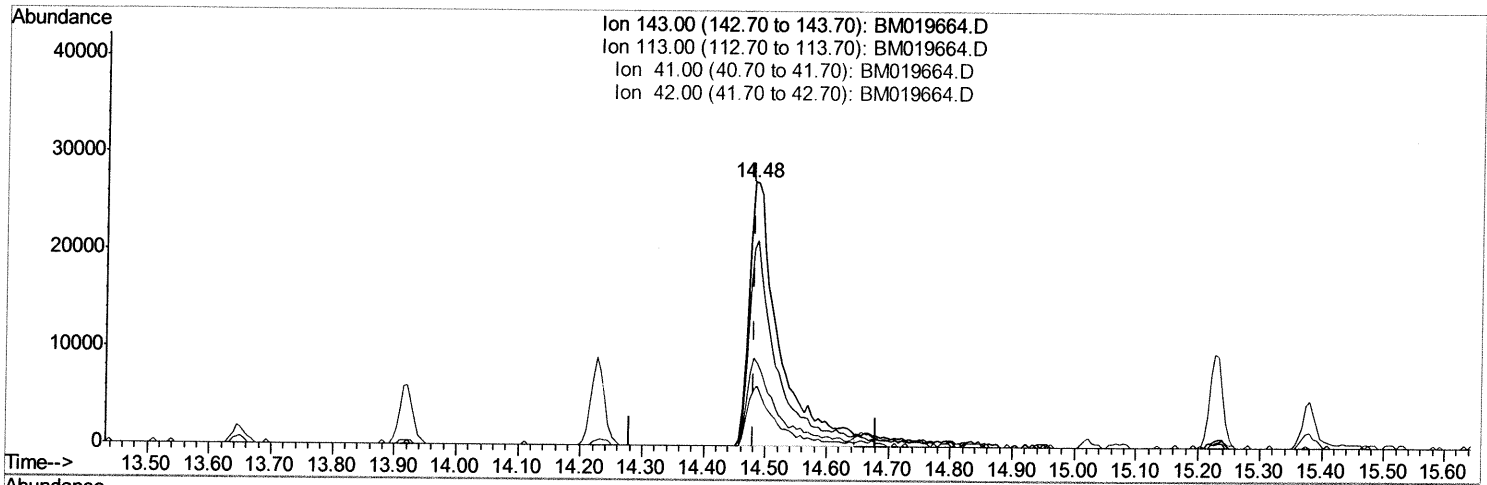

TIC: BM019664.D

(52) 4-Nitrophenol-d4 (S)

14.480min (0.000) 15.38ng/ul m 5] 4/3/19

response 92059

Ion	Exp%	Act%
143.00	100	100
113.00	77.10	74.47
41.00	32.60	33.00
42.00	22.30	21.01

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040119\
 Data File : BM019664.D
 Acq On : 01 Apr 2019 20:34
 Operator : JU/SJ
 Sample : K2119-14
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF5A9

Manual Integrations
 APPROVED

Sohil
 4/2/2019 5:31:14 PM

Quant Time: Apr 02 07:46:34 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 02 07:07:56 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	186305	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.35	136	820027	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.23	164	473207	20.00	ng/ul	-0.01
62) Phenanthrene-d10	16.99	188	1010407	20.00	ng/ul	-0.01
78) Chrysene-d12	21.20	240	997786	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	928732	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.12	96	28027	5.89	ng/uL	0.00
5) Phenol-d5	6.75	99	289195	17.43	ng/ul	-0.01
7) Bis-(2-Chloroethyl) ether-d	6.92	67	200496	18.05	ng/ul	-0.01
9) 2-Chlorophenol-d4	7.10	132	233409	18.56	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	240244	19.29	ng/ul	0.00
19) Nitrobenzene-d5	8.74	128	115762	19.79	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.45	143	131244	20.16	ng/ul	-0.01
26) 2,4-Dichlorophenol-d3	9.98	165	204207	16.62	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.52	131	300678	20.38	ng/ul	0.00
44) Dimethylphthalate-d6	13.65	166	801773	21.00	ng/ul	-0.01
47) Acenaphthylene-d8	13.92	160	925003	19.37	ng/ul	-0.01
52) 4-Nitrophenol-d4	14.48	143	92059m	15.38	ng/ul	0.00
58) Fluorene-d10	15.23	176	659739	20.05	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.38	200	99320	14.86	ng/ul	0.00
71) Anthracene-d10	17.09	188	1008256	20.79	ng/ul	-0.01
79) Pyrene-d10	19.40	212	1034779	22.45	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	915611	18.60	ng/ul	0.00

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.70	163	252077	6.580	ng/ul#	98

51 4/3/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed