

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM040119\
 Data File : BM019647.D
 Acq On : 01 Apr 2019 09:45
 Operator : JU/SJ
 Sample : K2065-05
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF5J6

Quant Time: Apr 02 03:59:30 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 02 03:56:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	122559	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.35	136	537787	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.23	164	296222	20.00	ng/ul	-0.01
62) Phenanthrene-d10	16.99	188	668172	20.00	ng/ul	-0.01
78) Chrysene-d12	21.20	240	805664	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	866184	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.12	96	20983	6.70	ng/uL	0.00
5) Phenol-d5	6.76	99	183182	16.78	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	129190	17.68	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	154789	18.71	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	126873	15.49	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	68895	17.96	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	73775	17.28	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	128519	15.95	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	153679	15.88	ng/ul	0.00
44) Dimethylphthalate-d6	13.65	166	465129	19.46	ng/ul	-0.01
47) Acenaphthylene-d8	13.92	160	532851	17.83	ng/ul	-0.01
52) 4-Nitrophenol-d4	14.49	143	47934	12.79	ng/ul	0.01
58) Fluorene-d10	15.23	176	397783	19.32	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.38	200	46734	10.58	ng/ul	0.00
71) Anthracene-d10	17.09	188	636234	19.84	ng/ul	0.00
79) Pyrene-d10	19.40	212	717800	19.29	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	834143	18.17	ng/ul	0.00

Target Compounds


					Ovalue
6) Phenol	6.78	94	11893	1.044 ng/ul#	80
45) Dimethylphthalate	13.70	163	63070	2.630 ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM040119\
Data File : BM019647.D
Acq On : 01 Apr 2019 09:45
Operator : JU/SJ
Sample : K2065-05
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF5J6

Quant Time: Apr 02 03:59:30 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 02 03:56:34 2019
Response via : Initial Calibration

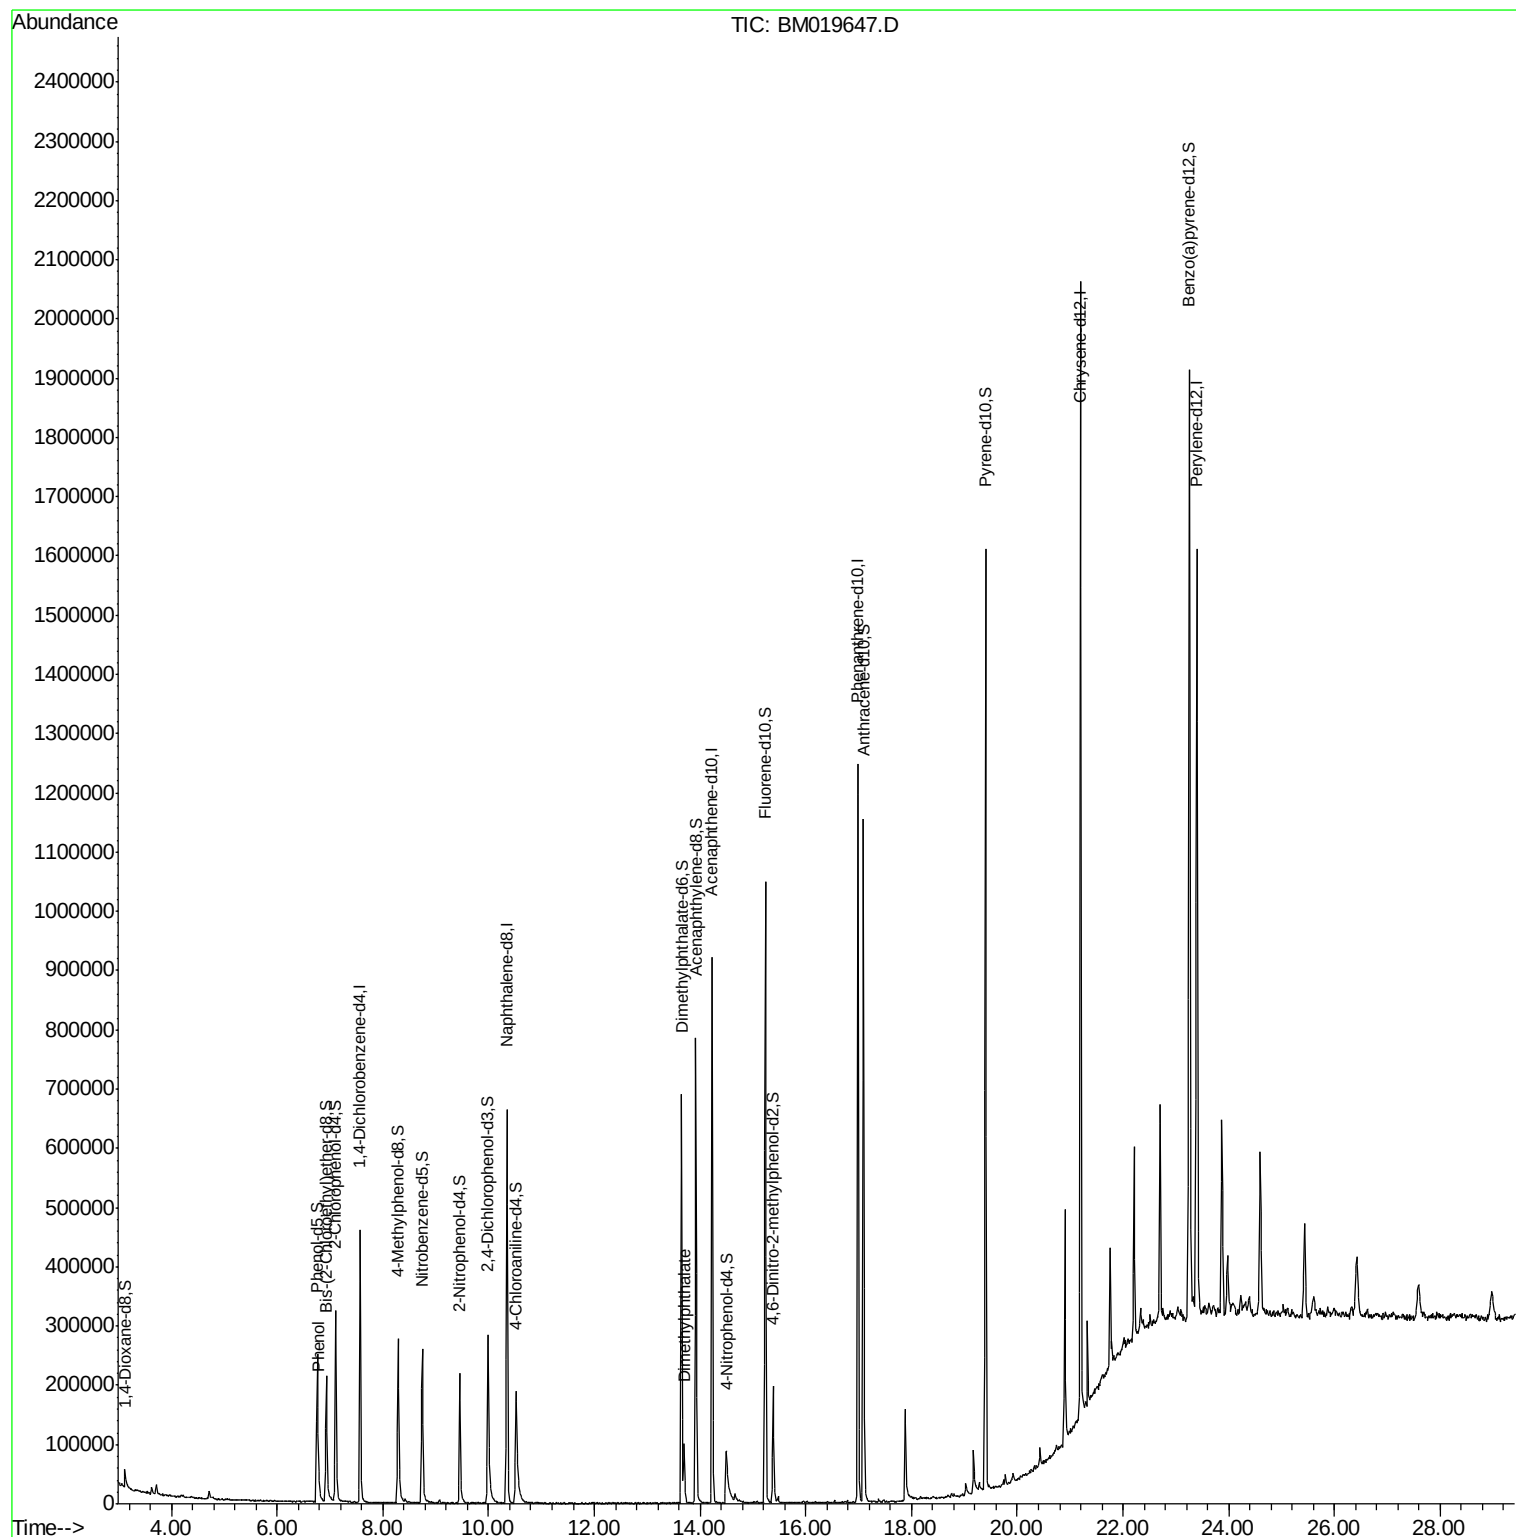

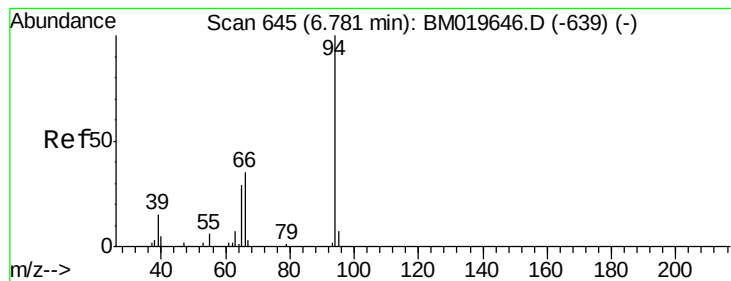





#6

Phenol

Concen: 1.044 ng/ul
 RT: 6.78 min Scan# 645
 Delta R.T. -0.01 min
 Lab File: BM019647.D
 Acq: 01 Apr 2019 09:45

Instrument :
 BNA_M
 ClientSampleId :
 BF5J6

Tot Ion	94	Resp	11893
Ion Ratio	Lower	Upper	
94	100		
65	32.2	23.0	34.6
66	55.9	30.4	45.6

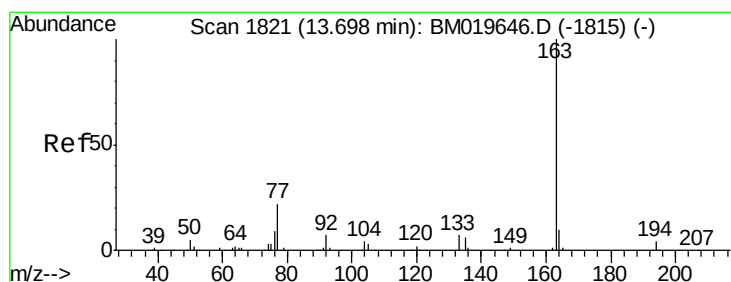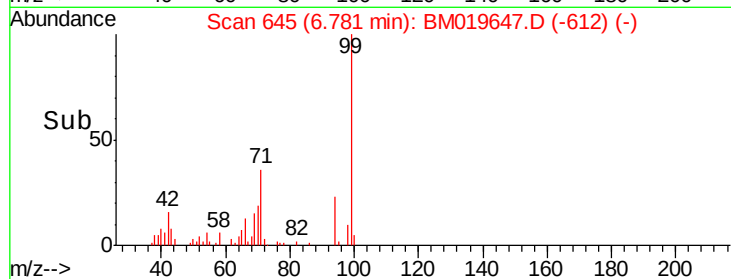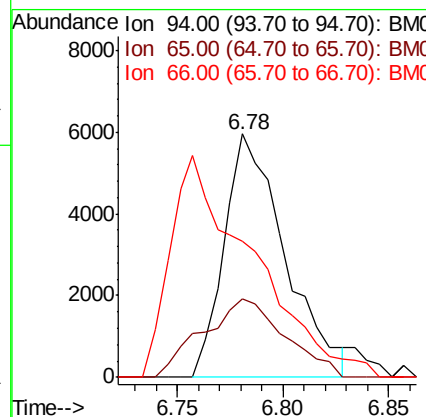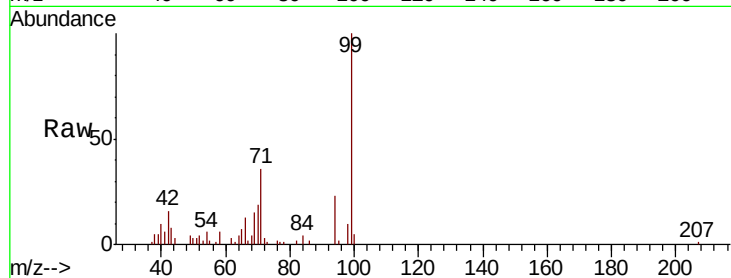

#45

Dimethylphthalate

Concen: 2.630 ng/ul
 RT: 13.70 min Scan# 1822
 Delta R.T. -0.01 min
 Lab File: BM019647.D
 Acq: 01 Apr 2019 09:45

Tgt Ion	163	Resp	63070
Ion Ratio	Lower	Upper	
163	100		
194	4.1	4.0	6.0
164	10.1	8.4	12.6

