

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM040119\
 Data File : BM019653.D
 Acq On : 01 Apr 2019 13:58
 Operator : JU/SJ
 Sample : K2119-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF598

Manual Integrations
 APPROVED

Sohil
 4/2/2019 5:31:05 PM

Quant Time: Apr 02 06:42:03 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 02 03:56:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	105459	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.35	136	473576	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.23	164	269102	20.00	ng/ul	-0.01
62) Phenanthrene-d10	16.99	188	620398	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	782935	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	905028	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	14343m	5.32	ng/uL	0.00
5) Phenol-d5	6.76	99	132711	14.13	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	86412	13.74	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	105728	14.85	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	99661	14.14	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	48728	14.42	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	54717	14.55	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	98640m	13.90	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	132687m	15.57	ng/ul	0.00
44) Dimethylphthalate-d6	13.65	166	343708	15.83	ng/ul	-0.01
47) Acenaphthylene-d8	13.92	160	401961	14.80	ng/ul	-0.01
52) 4-Nitrophenol-d4	14.50	143	36222m	10.64	ng/ul	0.02
58) Fluorene-d10	15.23	176	294343	15.73	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	27881	6.80	ng/ul	0.00
71) Anthracene-d10	17.09	188	461600	15.50	ng/ul	-0.01
79) Pyrene-d10	19.40	212	528625	14.62	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	653547	13.62	ng/ul	0.00

Target Compounds					Ovalue	
45) Dimethylphthalate	13.70	163	76544	3.513	ng/ul#	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM040119\
Data File : BM019653.D
Acq On : 01 Apr 2019 13:58
Operator : JU/SJ
Sample : K2119-01
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampled :
BF598

Quant Time: Apr 02 06:42:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 02 03:56:34 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
4/2/2019 5:31:05 PM

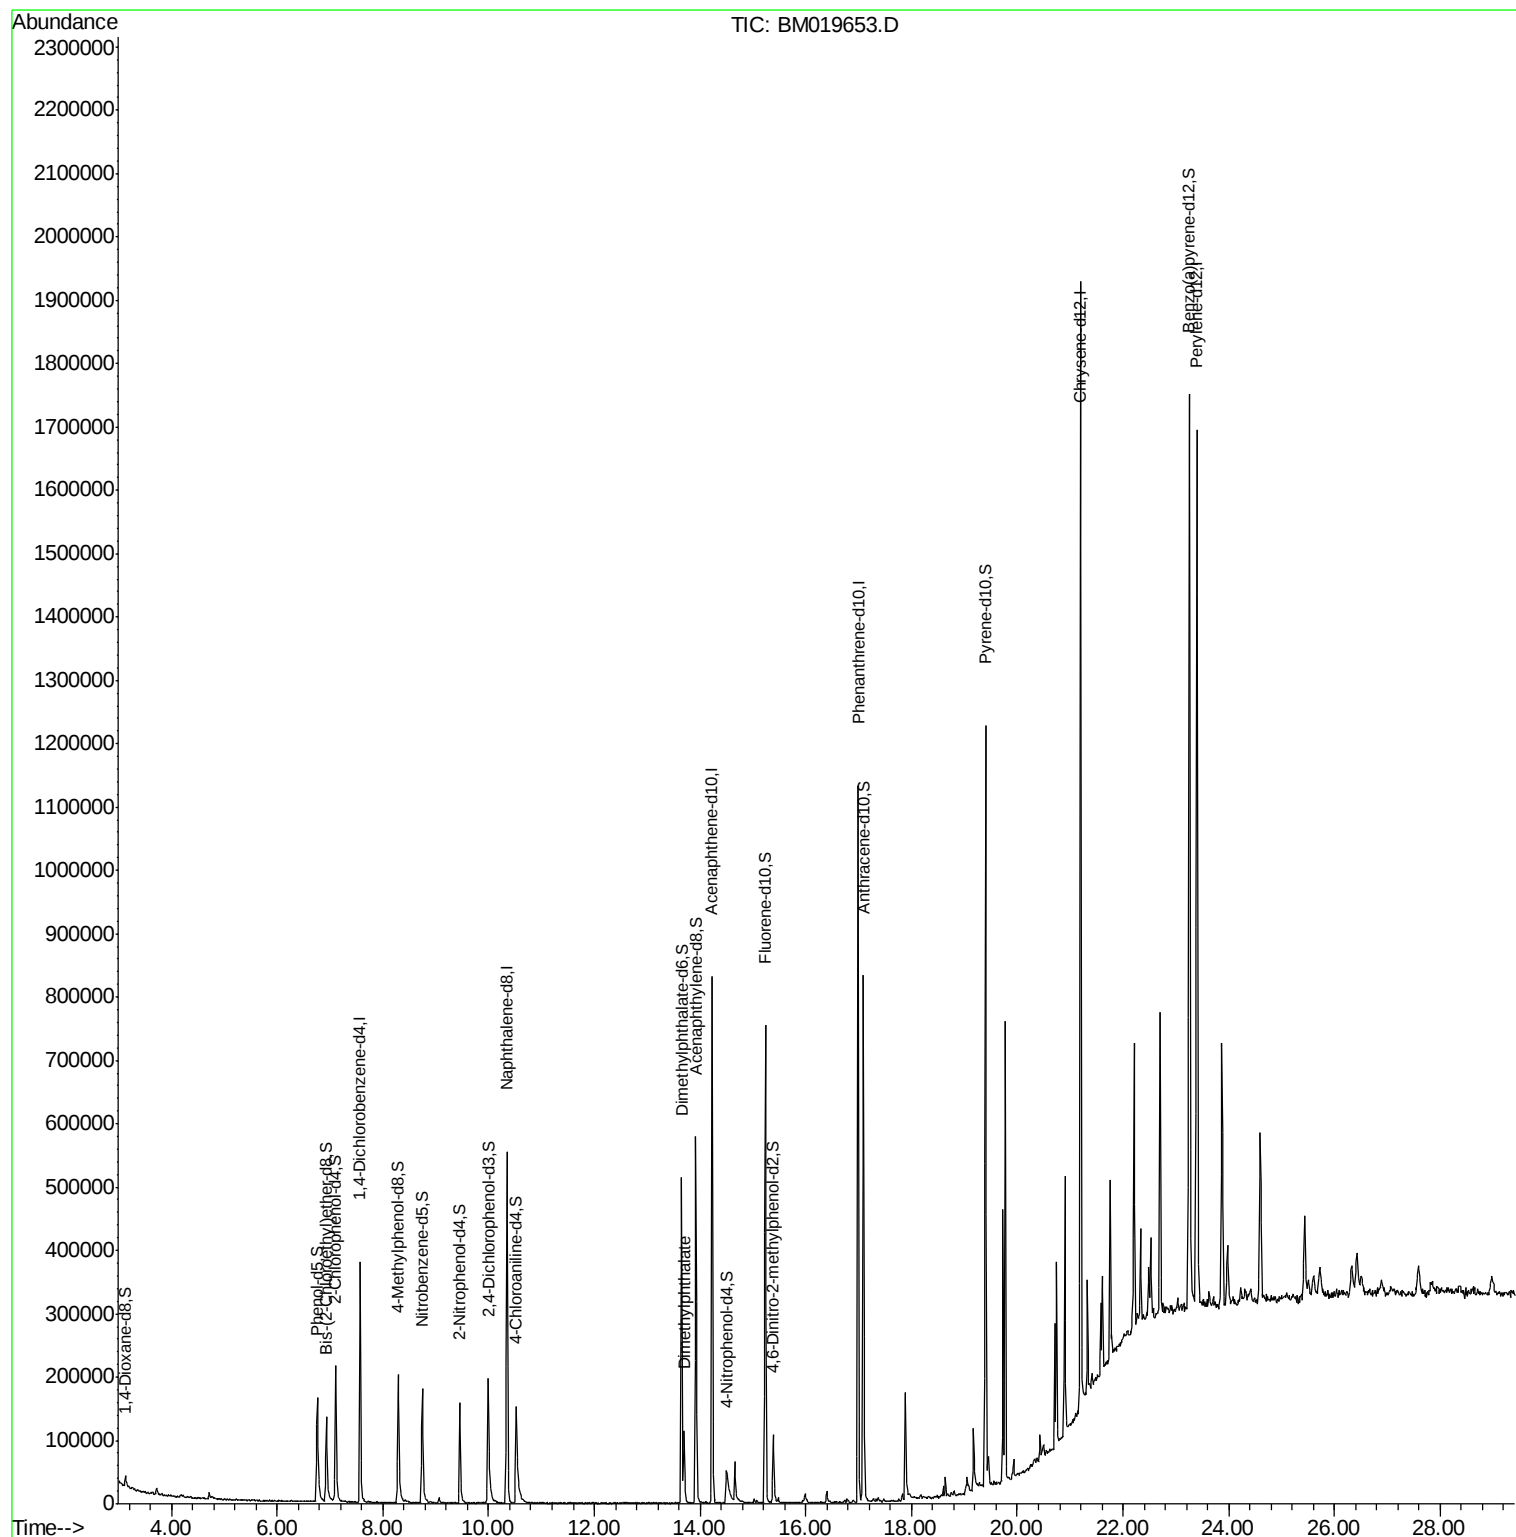

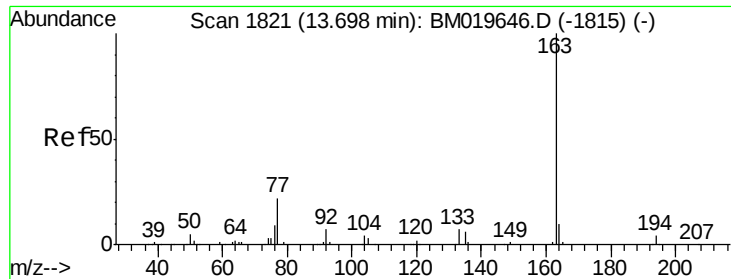

#45
 Dimethylphthalate
 Concen: 3.513 ng/ul
 RT: 13.70 min Scan# 1821
 Delta R.T. -0.01 min
 Lab File: BM019653.D
 Acq: 01 Apr 2019 13:58

Instrument :
 BNA_M
 ClientSampleId :
 BF598

Tot Ion	Ratio	Resp	Lower	Upper
163	100	76544		
194	4.0		4.0	6.0#
164	9.7		8.4	12.6

Manual Integrations
 APPROVED

Sohil
 4/2/2019 5:31:05 PM

