

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM040119\
 Data File : BM019654.D
 Acq On : 01 Apr 2019 14:34
 Operator : JU/SJ
 Sample : K2119-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF599

Manual Integrations
 APPROVED

Sohil
 4/2/2019 5:31:06 PM

Quant Time: Apr 02 06:47:17 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 02 03:56:34 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	117874	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.35	136	531391	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.23	164	299672	20.00	ng/ul	-0.01
62) Phenanthrene-d10	16.99	188	692266	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	875613	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	968937	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.12	96	18723	6.22	ng/uL	0.00
5) Phenol-d5	6.76	99	192350	18.32	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.93	67	134625	19.16	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	161777	20.34	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	158241	20.08	ng/ul	0.00
19) Nitrobenzene-d5	8.74	128	74091	19.55	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.45	143	83280	19.74	ng/ul	-0.01
26) 2,4-Dichlorophenol-d3	9.99	165	140780	17.69	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	186502	19.51	ng/ul	0.00
44) Dimethylphthalate-d6	13.65	166	501773	20.75	ng/ul	-0.01
47) Acenaphthylene-d8	13.92	160	582392	19.26	ng/ul	-0.01
52) 4-Nitrophenol-d4	14.50	143	54927m	14.49	ng/ul	0.02
58) Fluorene-d10	15.23	176	417377	20.03	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.38	200	49763	10.87	ng/ul	0.00
71) Anthracene-d10	17.09	188	671774	20.22	ng/ul	-0.01
79) Pyrene-d10	19.40	212	755353	18.68	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	924145	17.99	ng/ul	-0.01

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.70	163	80749	3.328	ng/ul#	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM040119\
Data File : BM019654.D
Acq On : 01 Apr 2019 14:34
Operator : JU/SJ
Sample : K2119-02
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BF599

Quant Time: Apr 02 06:47:17 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 02 03:56:34 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
4/2/2019 5:31:06 PM

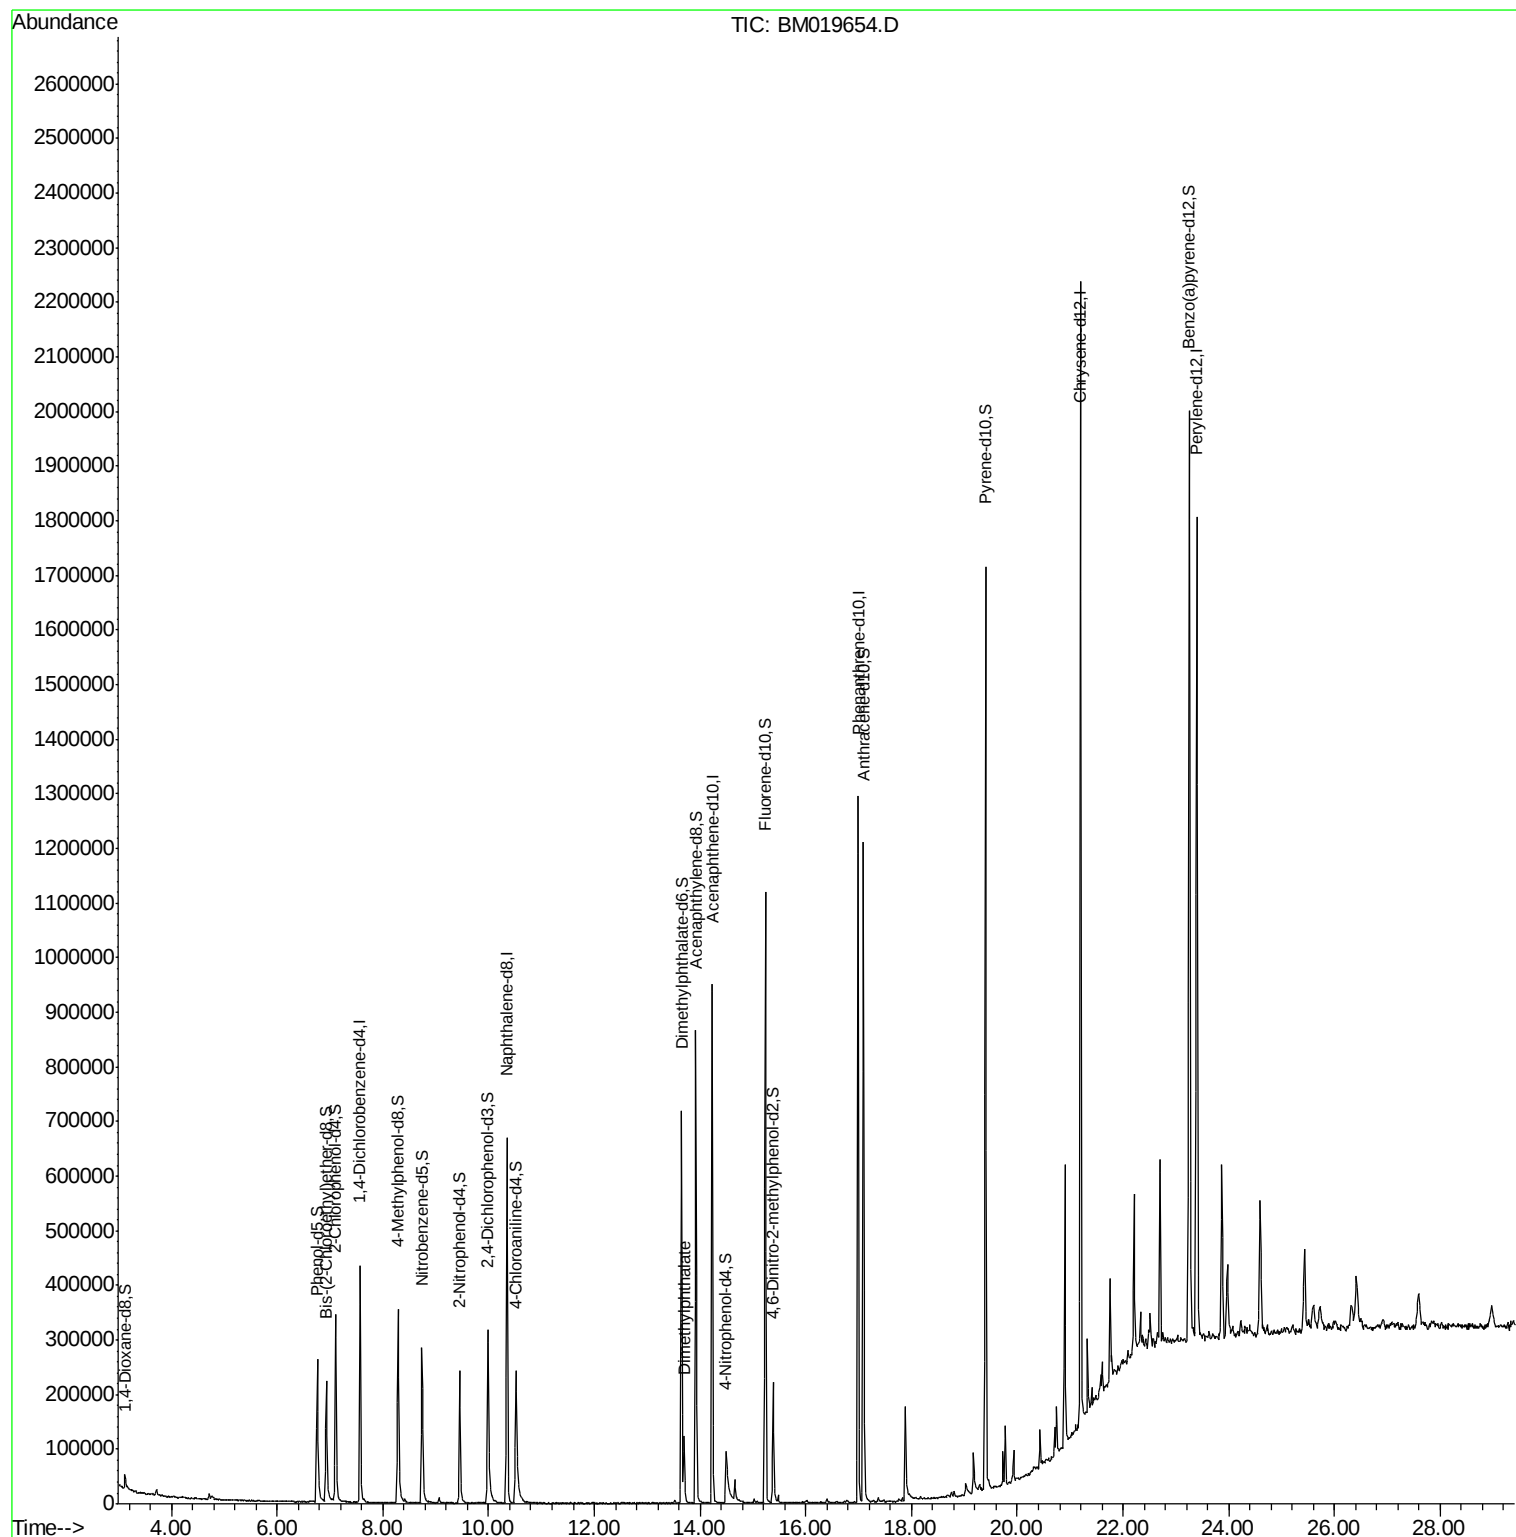

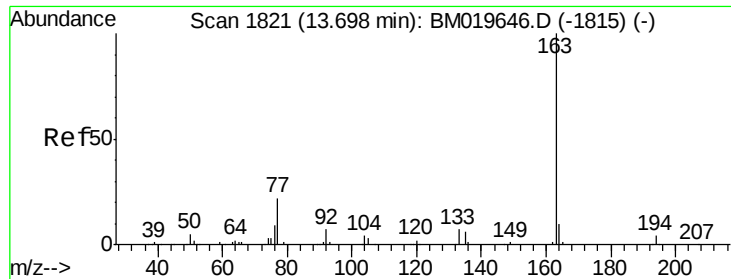

#45
 Dimethylphthalate
 Concen: 3.328 ng/ul
 RT: 13.70 min Scan# 1822
 Delta R.T. -0.01 min
 Lab File: BM019654.D
 Acq: 01 Apr 2019 14:34

Instrument :
 BNA_M
 ClientSampleId :
 BF599

Tot Ion	Ratio	Resp	Lower	Upper
163	100	80749		
194	3.9		4.0	6.0#
164	10.5		8.4	12.6

Manual Integrations
 APPROVED

Sohil
 4/2/2019 5:31:06 PM

