

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM040119\
 Data File : BM019659.D
 Acq On : 01 Apr 2019 17:34
 Operator : JU/SJ
 Sample : K2119-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF5A3

Quant Time: Apr 02 07:10:45 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 02 07:07:56 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	173830	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.35	136	775040	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.23	164	451673	20.00	ng/ul	-0.01
62) Phenanthrene-d10	16.99	188	1000769	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	978632	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	928388	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.12	96	25655	5.78	ng/uL	0.00
5) Phenol-d5	6.75	99	345543	22.32	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	6.92	67	231817	22.37	ng/ul	-0.01
9) 2-Chlorophenol-d4	7.10	132	276358	23.56	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	285643	24.58	ng/ul	-0.01
19) Nitrobenzene-d5	8.74	128	132338	23.94	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.45	143	153669	24.97	ng/ul	-0.01
26) 2,4-Dichlorophenol-d3	9.98	165	262376	22.60	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.52	131	358503	25.71	ng/ul	0.00
44) Dimethylphthalate-d6	13.65	166	945697	25.95	ng/ul	-0.01
47) Acenaphthylene-d8	13.92	160	1156222	25.37	ng/ul	-0.01
52) 4-Nitrophenol-d4	14.48	143	114772	20.09	ng/ul	0.00
58) Fluorene-d10	15.23	176	797927	25.41	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.38	200	117213	17.71	ng/ul	0.00
71) Anthracene-d10	17.09	188	1229234	25.60	ng/ul	0.00
79) Pyrene-d10	19.40	212	1310502	28.99	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	1193605	24.25	ng/ul	0.00


Target Compounds				Ovalue	
45) Dimethylphthalate	13.70	163	248727	6.802	ng/ul# 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM040119\
Data File : BM019659.D
Acq On : 01 Apr 2019 17:34
Operator : JU/SJ
Sample : K2119-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF5A3

Quant Time: Apr 02 07:10:45 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 02 07:07:56 2019
Response via : Initial Calibration

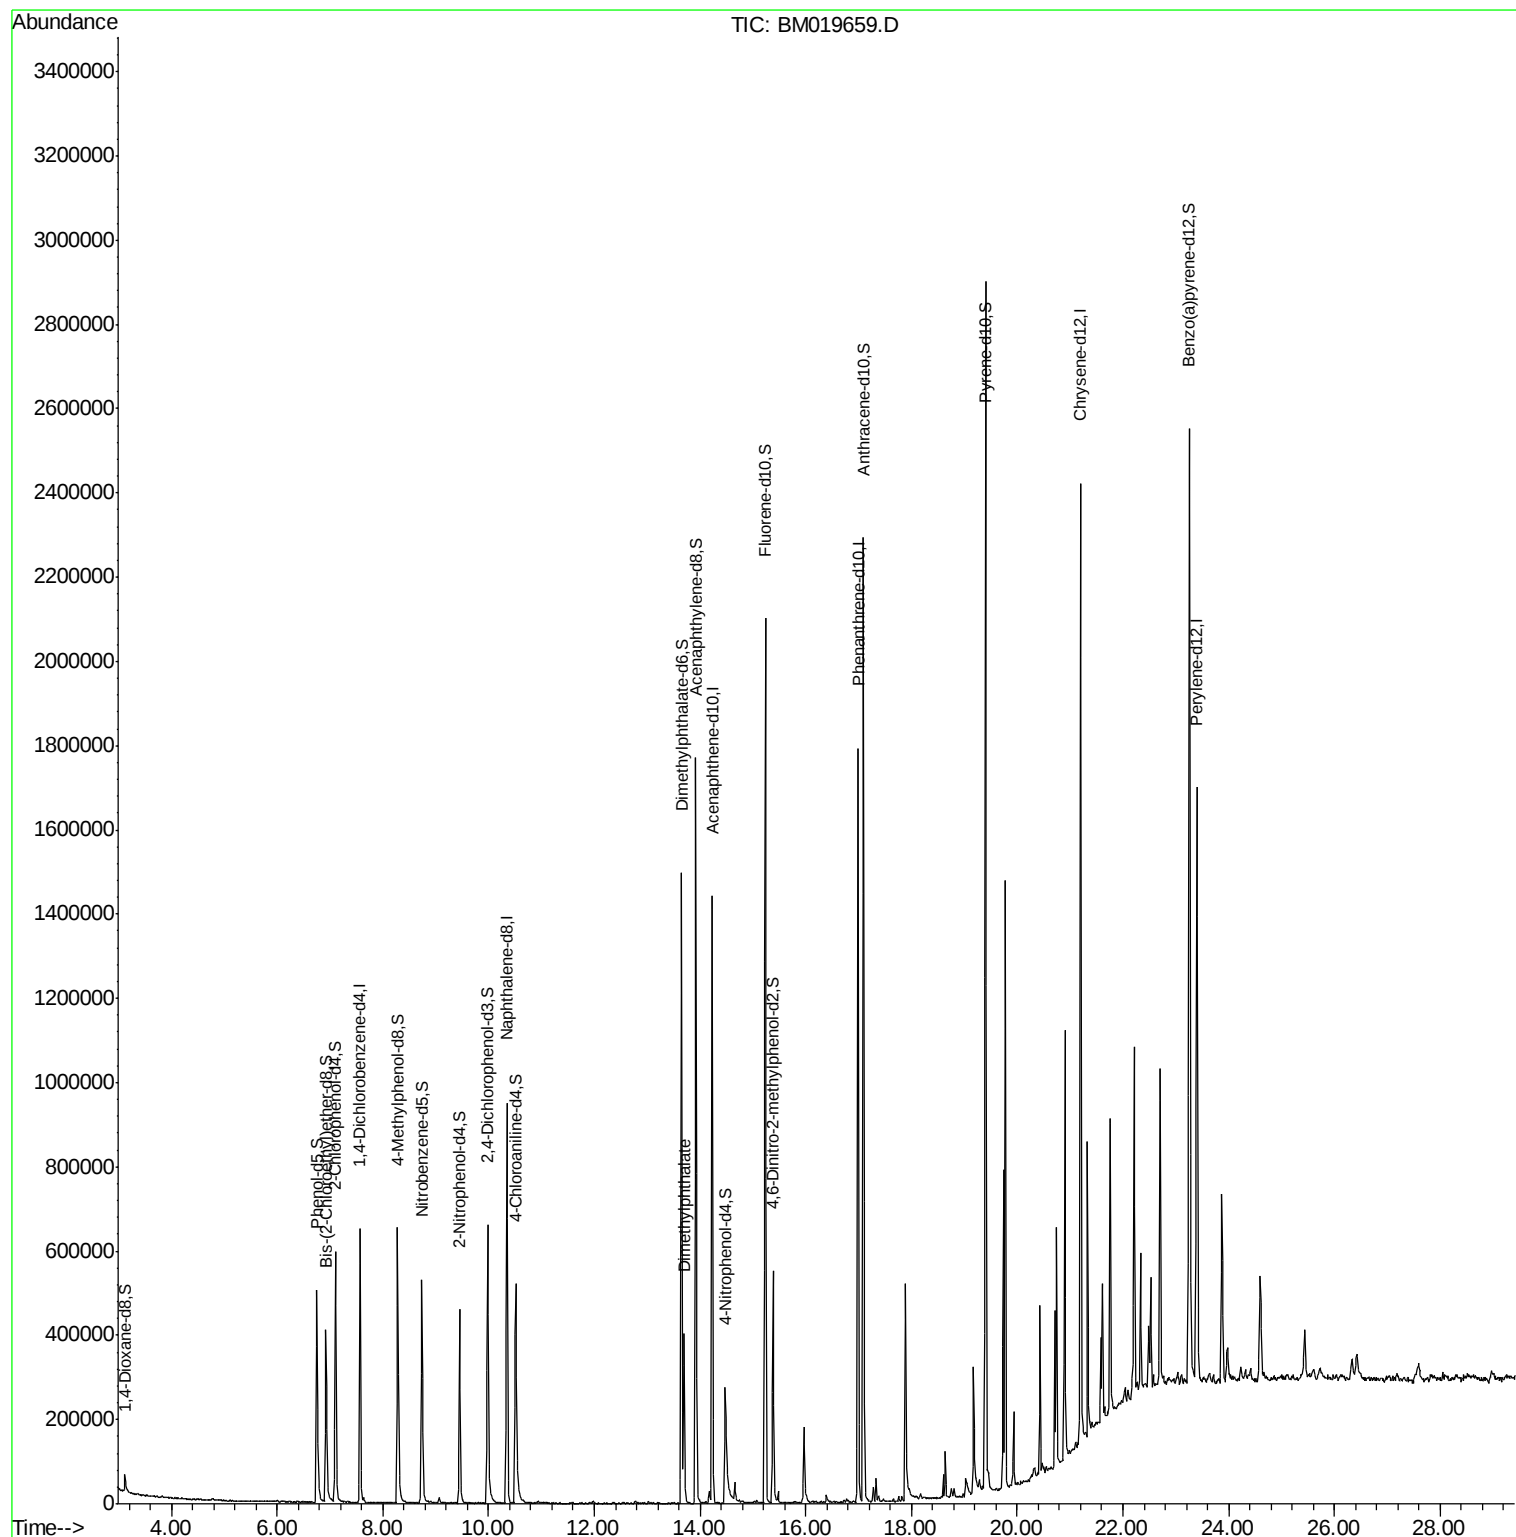

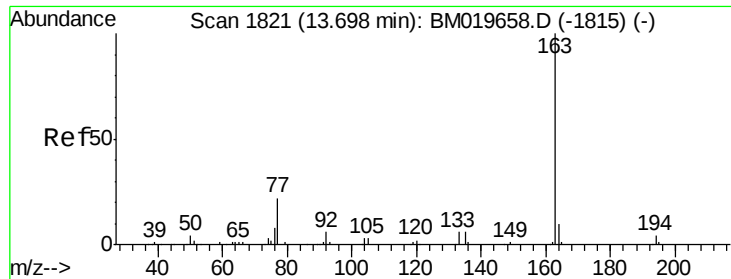

#45

Dimethylphthalate

Concen: 6.802 ng/ul

RT: 13.70 min Scan# 1821

Delta R.T. -0.01 min

Lab File: BM019659.D

Acq: 01 Apr 2019 17:34

Instrument :

BNA_M

ClientSampleId :

BF5A3


Tot Ion:163 Resp: 248727

Ion Ratio Lower Upper

163 100

194 3.7 4.0 6.0#

164 10.2 8.4 12.6

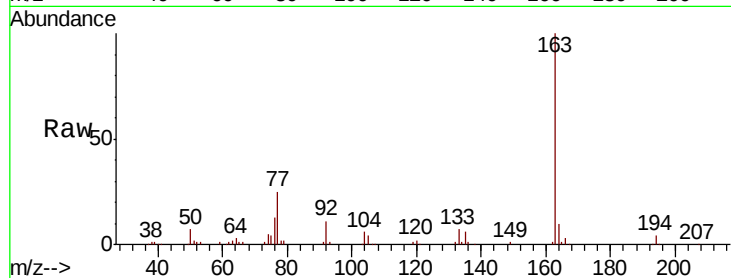

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

