

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM040119\
 Data File : BM019662.D
 Acq On : 01 Apr 2019 19:22
 Operator : JU/SJ
 Sample : K2119-11
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF5A5

Manual Integrations
 APPROVED

Sohil
 4/2/2019 5:31:13 PM

Quant Time: Apr 02 07:39:41 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 02 07:07:56 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	176570	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.35	136	777818	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.23	164	449959	20.00	ng/ul	-0.01
62) Phenanthrene-d10	16.99	188	987756	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	877683	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	815845	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.12	96	23685	5.25	ng/uL	0.00
5) Phenol-d5	6.76	99	242068	15.39	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	159974	15.20	ng/ul	-0.01
9) 2-Chlorophenol-d4	7.10	132	191621	16.08	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	196937	16.69	ng/ul	0.00
19) Nitrobenzene-d5	8.74	128	87170	15.71	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.45	143	97779	15.83	ng/ul	-0.01
26) 2,4-Dichlorophenol-d3	9.99	165	172231	14.78	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	188689	13.48	ng/ul	0.00
44) Dimethylphthalate-d6	13.65	166	643131	17.71	ng/ul	-0.01
47) Acenaphthylene-d8	13.92	160	723049	15.93	ng/ul	-0.01
52) 4-Nitrophenol-d4	14.49	143	84868m	14.91	ng/ul	0.00
58) Fluorene-d10	15.23	176	526293	16.82	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.38	200	80764	12.36	ng/ul	0.00
71) Anthracene-d10	17.09	188	856795	18.08	ng/ul	0.00
79) Pyrene-d10	19.40	212	922567	22.76	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	763789	17.66	ng/ul	0.00

Target Compounds					Ovalue
45) Dimethylphthalate	13.70	163	195680	5.372	ng/ul 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM040119\
Data File : BM019662.D
Acq On : 01 Apr 2019 19:22
Operator : JU/SJ
Sample : K2119-11
Misc :
ALS Vial : 17 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BF5A5

Manual Integrations
APPROVED

Sohil
4/2/2019 5:31:13 PM

Quant Time: Apr 02 07:39:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 02 07:07:56 2019
Response via : Initial Calibration

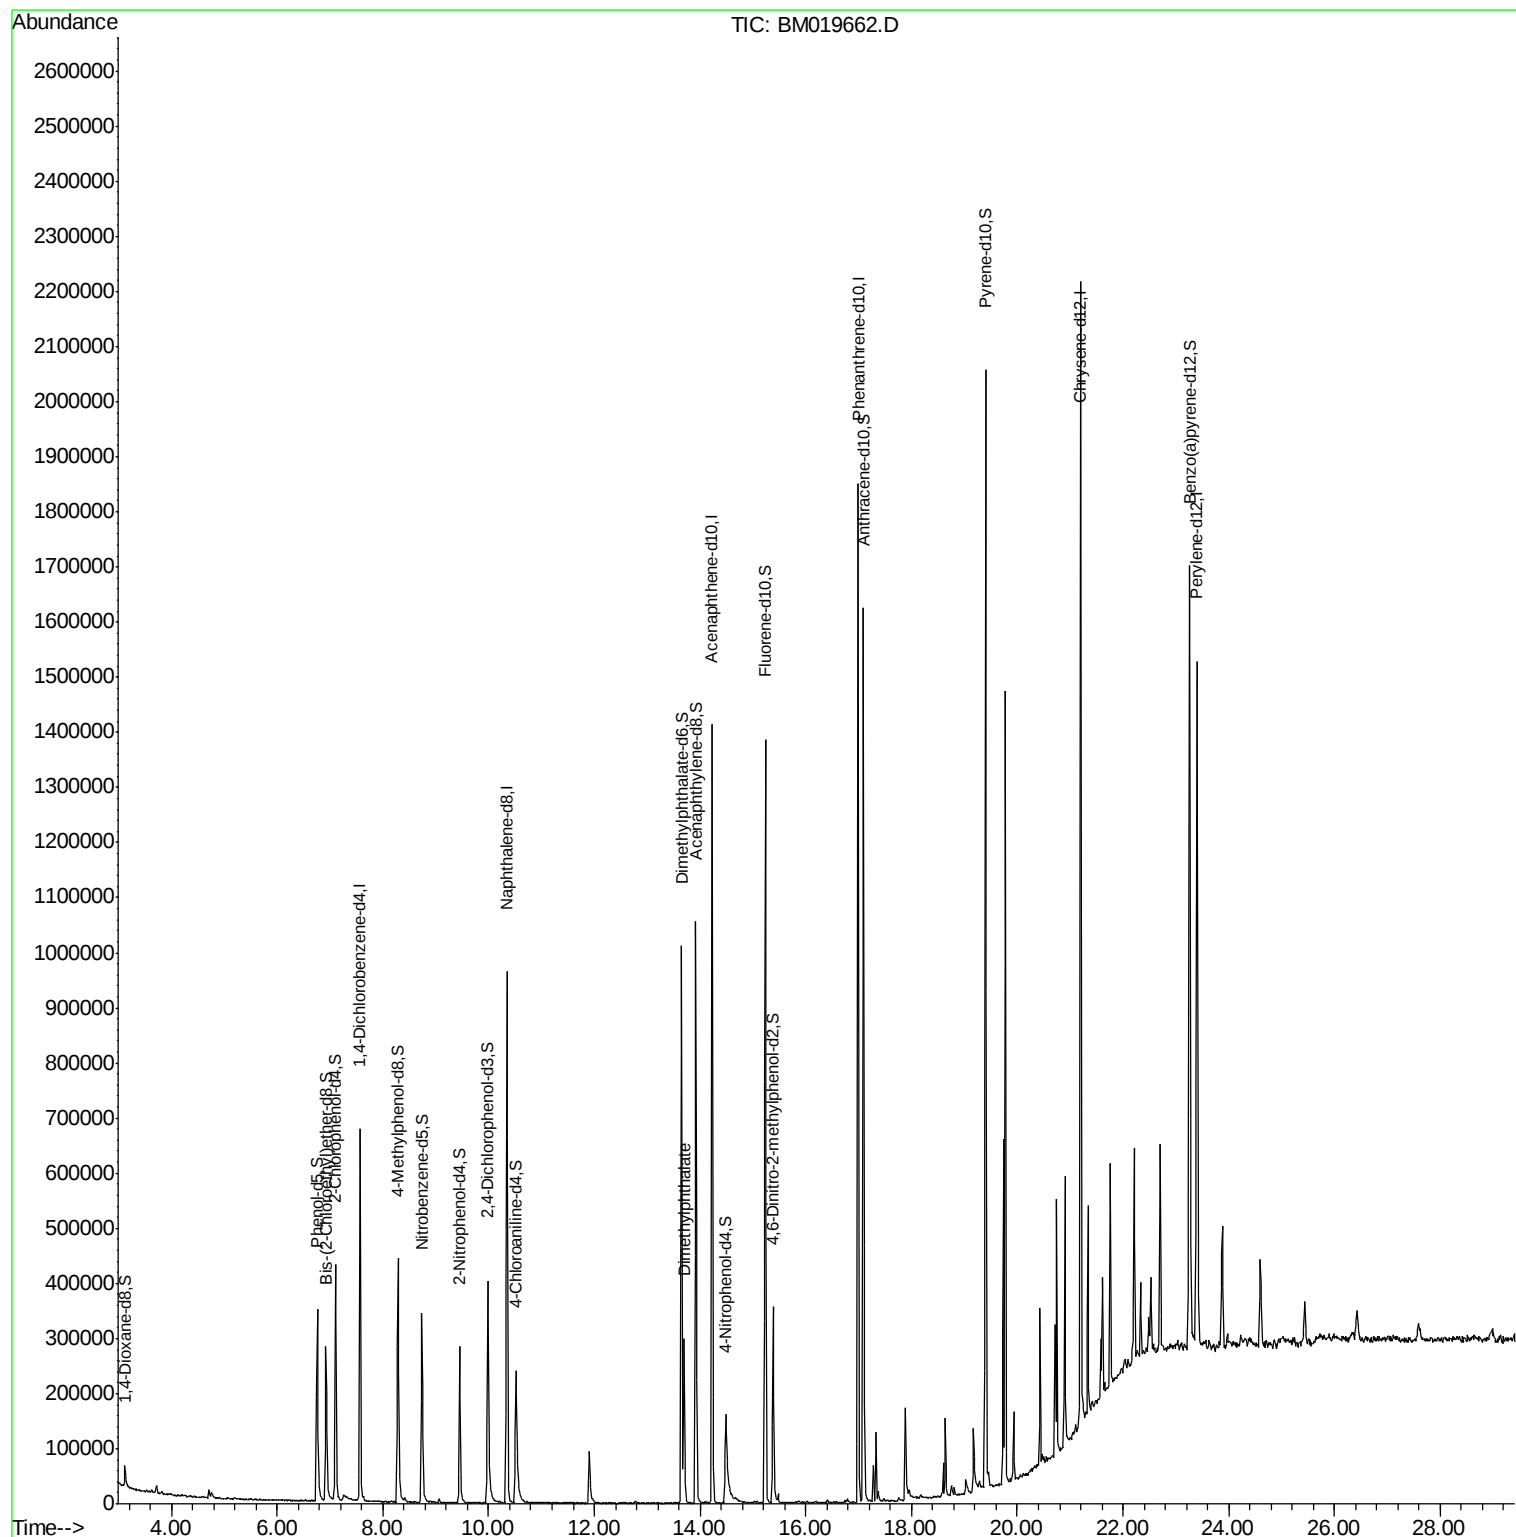

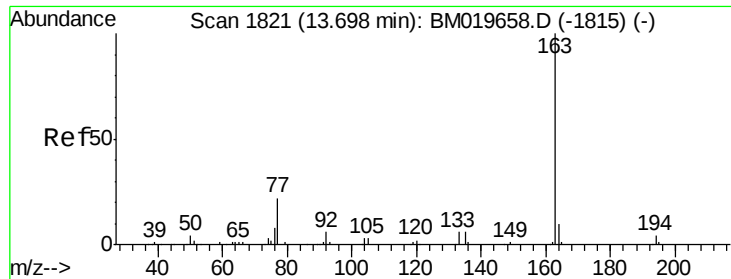

#45
 Dimethylphthalate
 Concen: 5.372 ng/ul
 RT: 13.70 min Scan# 1821
 Delta R.T. -0.01 min
 Lab File: BM019662.D
 Acq: 01 Apr 2019 19:22

Instrument :
 BNA_M
 ClientSampleId :
 BF5A5

Tot Ion:	163	Resp:	195680
Ion Ratio		Lower	Upper
163	100		
194	4.4	4.0	6.0
164	10.3	8.4	12.6

Manual Integrations
 APPROVED

Sohil
 4/2/2019 5:31:13 PM

