

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM040119\
 Data File : BM019663.D
 Acq On : 01 Apr 2019 19:58
 Operator : JU/SJ
 Sample : K2119-12
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF5A7

Quant Time: Apr 02 07:11:03 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 02 07:07:56 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	178203	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.35	136	816106	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.23	164	471507	20.00	ng/ul	-0.01
62) Phenanthrene-d10	16.99	188	1039877	20.00	ng/ul	-0.01
78) Chrysene-d12	21.20	240	985899	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	919811	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.12	96	24244	5.33	ng/uL	0.00
5) Phenol-d5	6.76	99	202801	12.78	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	146888	13.83	ng/ul	-0.01
9) 2-Chlorophenol-d4	7.10	132	166505	13.84	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	167403	14.05	ng/ul	0.00
19) Nitrobenzene-d5	8.74	128	78411	13.47	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.46	143	91271	14.09	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	158644	12.98	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	213830	14.56	ng/ul	0.00
44) Dimethylphthalate-d6	13.65	166	590846	15.53	ng/ul	-0.01
47) Acenaphthylene-d8	13.92	160	664115	13.96	ng/ul	-0.01
52) 4-Nitrophenol-d4	14.49	143	59959	10.05	ng/ul	0.01
58) Fluorene-d10	15.23	176	491656	15.00	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.38	200	65179	9.48	ng/ul	0.00
71) Anthracene-d10	17.09	188	766172	15.35	ng/ul	-0.01
79) Pyrene-d10	19.40	212	785026	17.24	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	667267	13.68	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.70	163	194373	5.092	ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM040119\
Data File : BM019663.D
Acq On : 01 Apr 2019 19:58
Operator : JU/SJ
Sample : K2119-12
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF5A7

Quant Time: Apr 02 07:11:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 02 07:07:56 2019
Response via : Initial Calibration

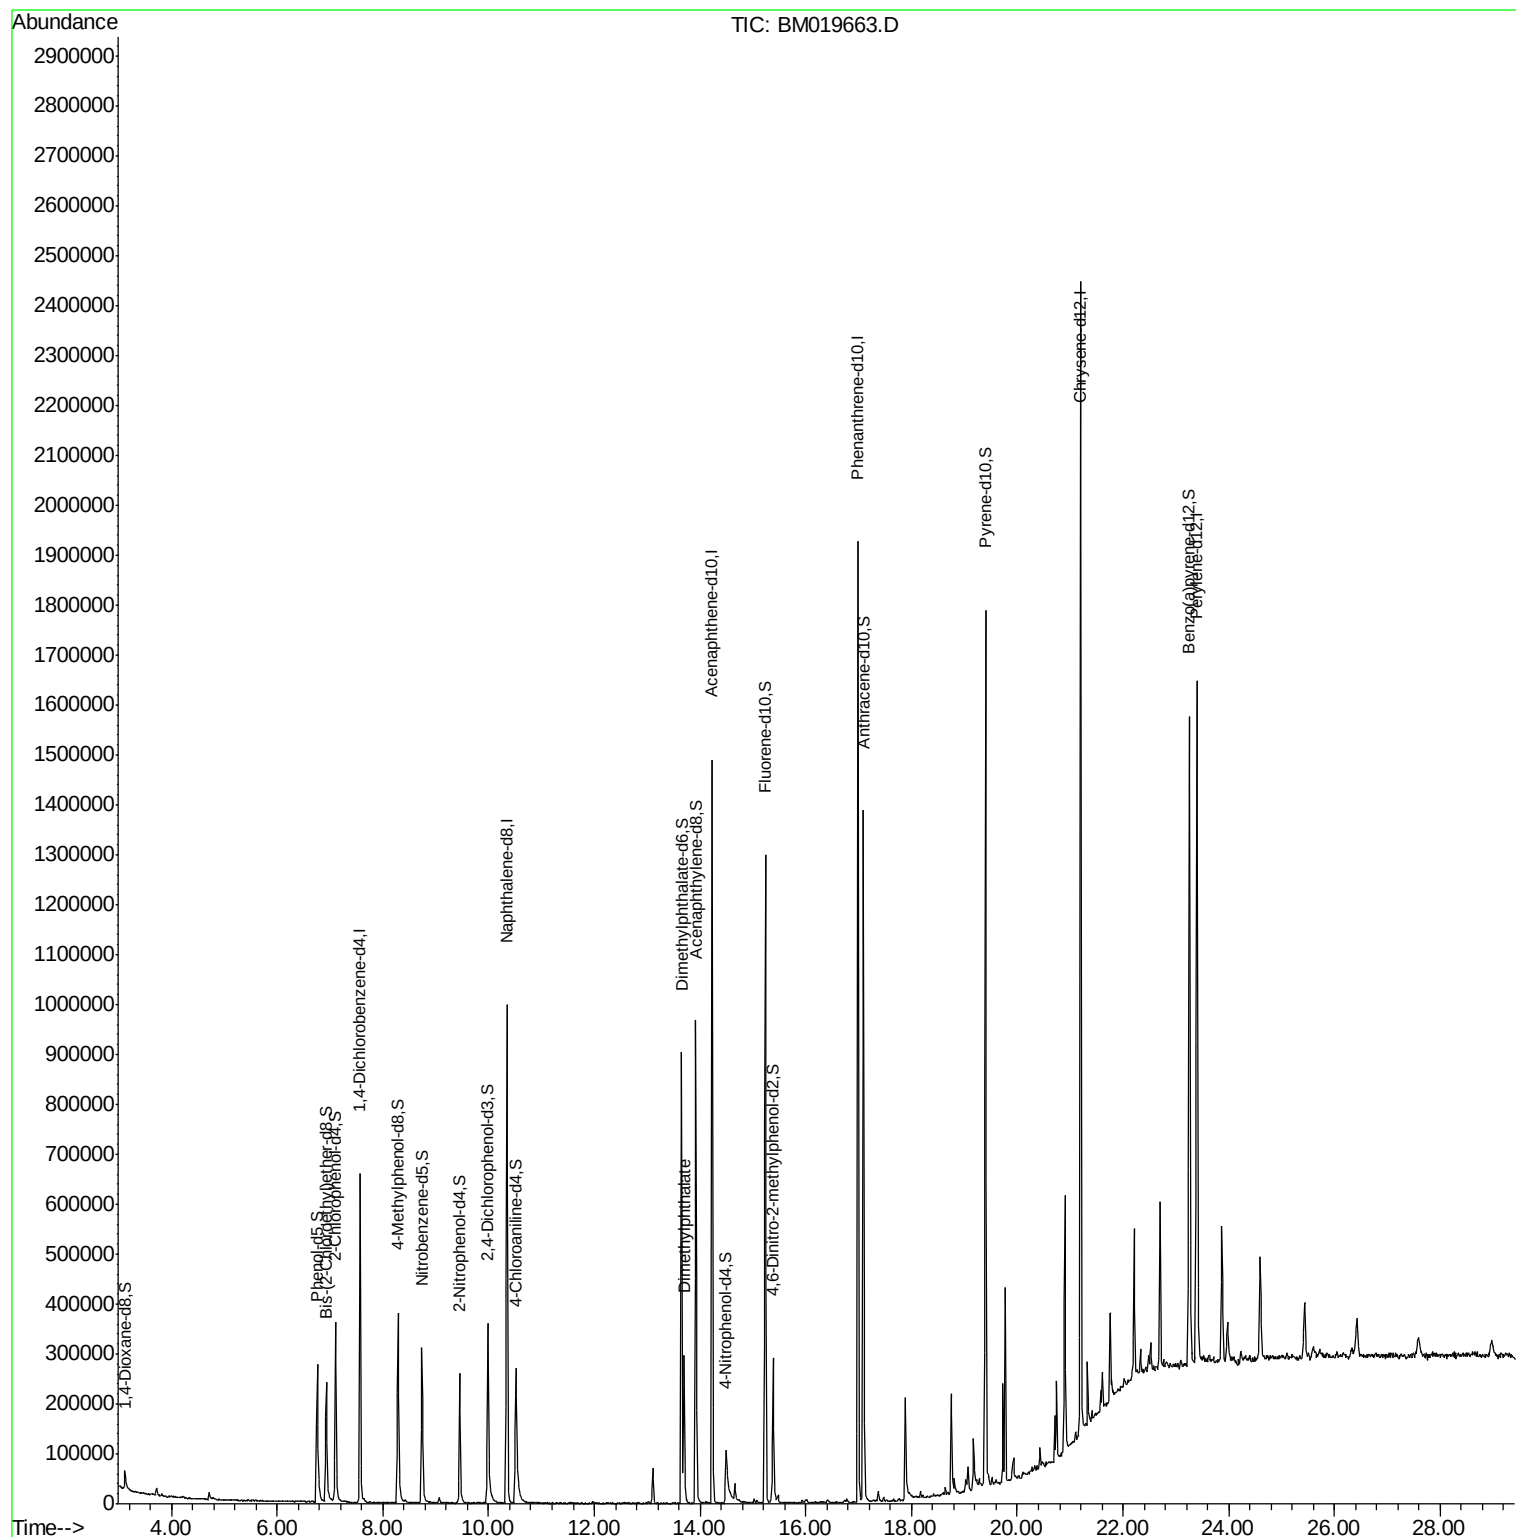

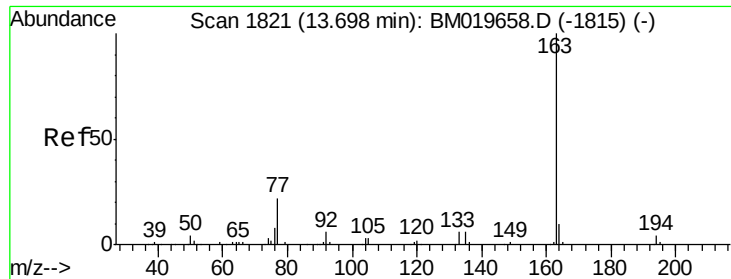

#45

Dimethylphthalate

Concen: 5.092 ng/ul

RT: 13.70 min Scan# 1821

Delta R.T. -0.01 min

Lab File: BM019663.D

Acq: 01 Apr 2019 19:58

Instrument :

BNA_M

ClientSampleId :

BF5A7


Tot Ion:163 Resp: 194373

Ion Ratio Lower Upper

163 100

194 3.6 4.0 6.0#

164 10.3 8.4 12.6

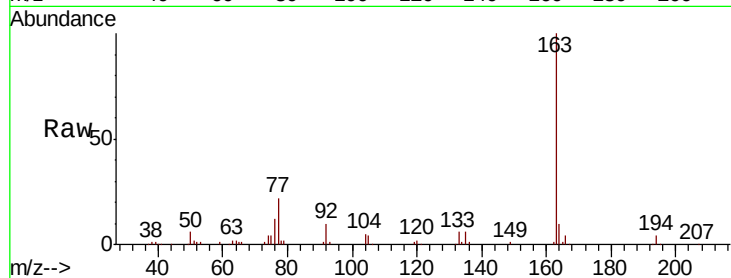

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

