

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM040119\
 Data File : BM019683.D
 Acq On : 02 Apr 2019 08:10
 Operator : JU/SJ
 Sample : K2068-21
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF5J9

Quant Time: Apr 02 11:23:03 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 28 05:07:19 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	226649	20.00	ng/ul	-0.03
18) Naphthalene-d8	10.35	136	969494	20.00	ng/ul	-0.03
36) Acenaphthene-d10	14.23	164	524049	20.00	ng/ul	-0.02
62) Phenanthrene-d10	17.00	188	981755	20.00	ng/ul	-0.02
78) Chrysene-d12	21.20	240	742297	20.00	ng/ul	-0.02
86) Perylene-d12	23.42	264	874511	20.00	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.12	96	30302	5.23	ng/uL	-0.02
5) Phenol-d5	6.76	99	322122	15.96	ng/ul	-0.02
7) Bis-(2-Chloroethyl)ether-d	6.93	67	221020	16.36	ng/ul	-0.02
9) 2-Chlorophenol-d4	7.11	132	270636	17.69	ng/ul	-0.02
13) 4-Methylphenol-d8	8.29	113	257539	17.00	ng/ul	-0.02
19) Nitrobenzene-d5	8.75	128	126819	18.34	ng/ul	-0.02
22) 2-Nitrophenol-d4	9.46	143	118516	15.40	ng/ul	-0.02
26) 2,4-Dichlorophenol-d3	9.99	165	255040	17.56	ng/ul	-0.02
29) 4-Chloroaniline-d4	10.52	131	241251	13.83	ng/ul	-0.02
44) Dimethylphthalate-d6	13.66	166	816227	19.30	ng/ul	-0.02
47) Acenaphthylene-d8	13.93	160	974084	18.42	ng/ul	-0.02
52) 4-Nitrophenol-d4	14.50	143	68703	10.37	ng/ul	0.00
58) Fluorene-d10	15.24	176	662889	18.20	ng/ul	-0.02
63) 4,6-Dinitro-2-methylphenol	15.41	200	772	0.12	ng/ul	0.00
71) Anthracene-d10	17.10	188	876809	18.61	ng/ul	-0.02
79) Pyrene-d10	19.40	212	694984	20.27	ng/ul	-0.02
90) Benzo(a)pyrene-d12	23.27	264	754457	16.27	ng/ul	-0.02
Target Compounds						
45) Dimethylphthalate	13.70	163	98799	2.329	ng/ul	97
84) Bis(2-ethylhexyl)phthalate	21.11	149	51292	2.001	ng/ul#	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM040119\
Data File : BM019683.D
Acq On : 02 Apr 2019 08:10
Operator : JU/SJ
Sample : K2068-21
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF5J9

Quant Time: Apr 02 11:23:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 28 05:07:19 2019
Response via : Initial Calibration

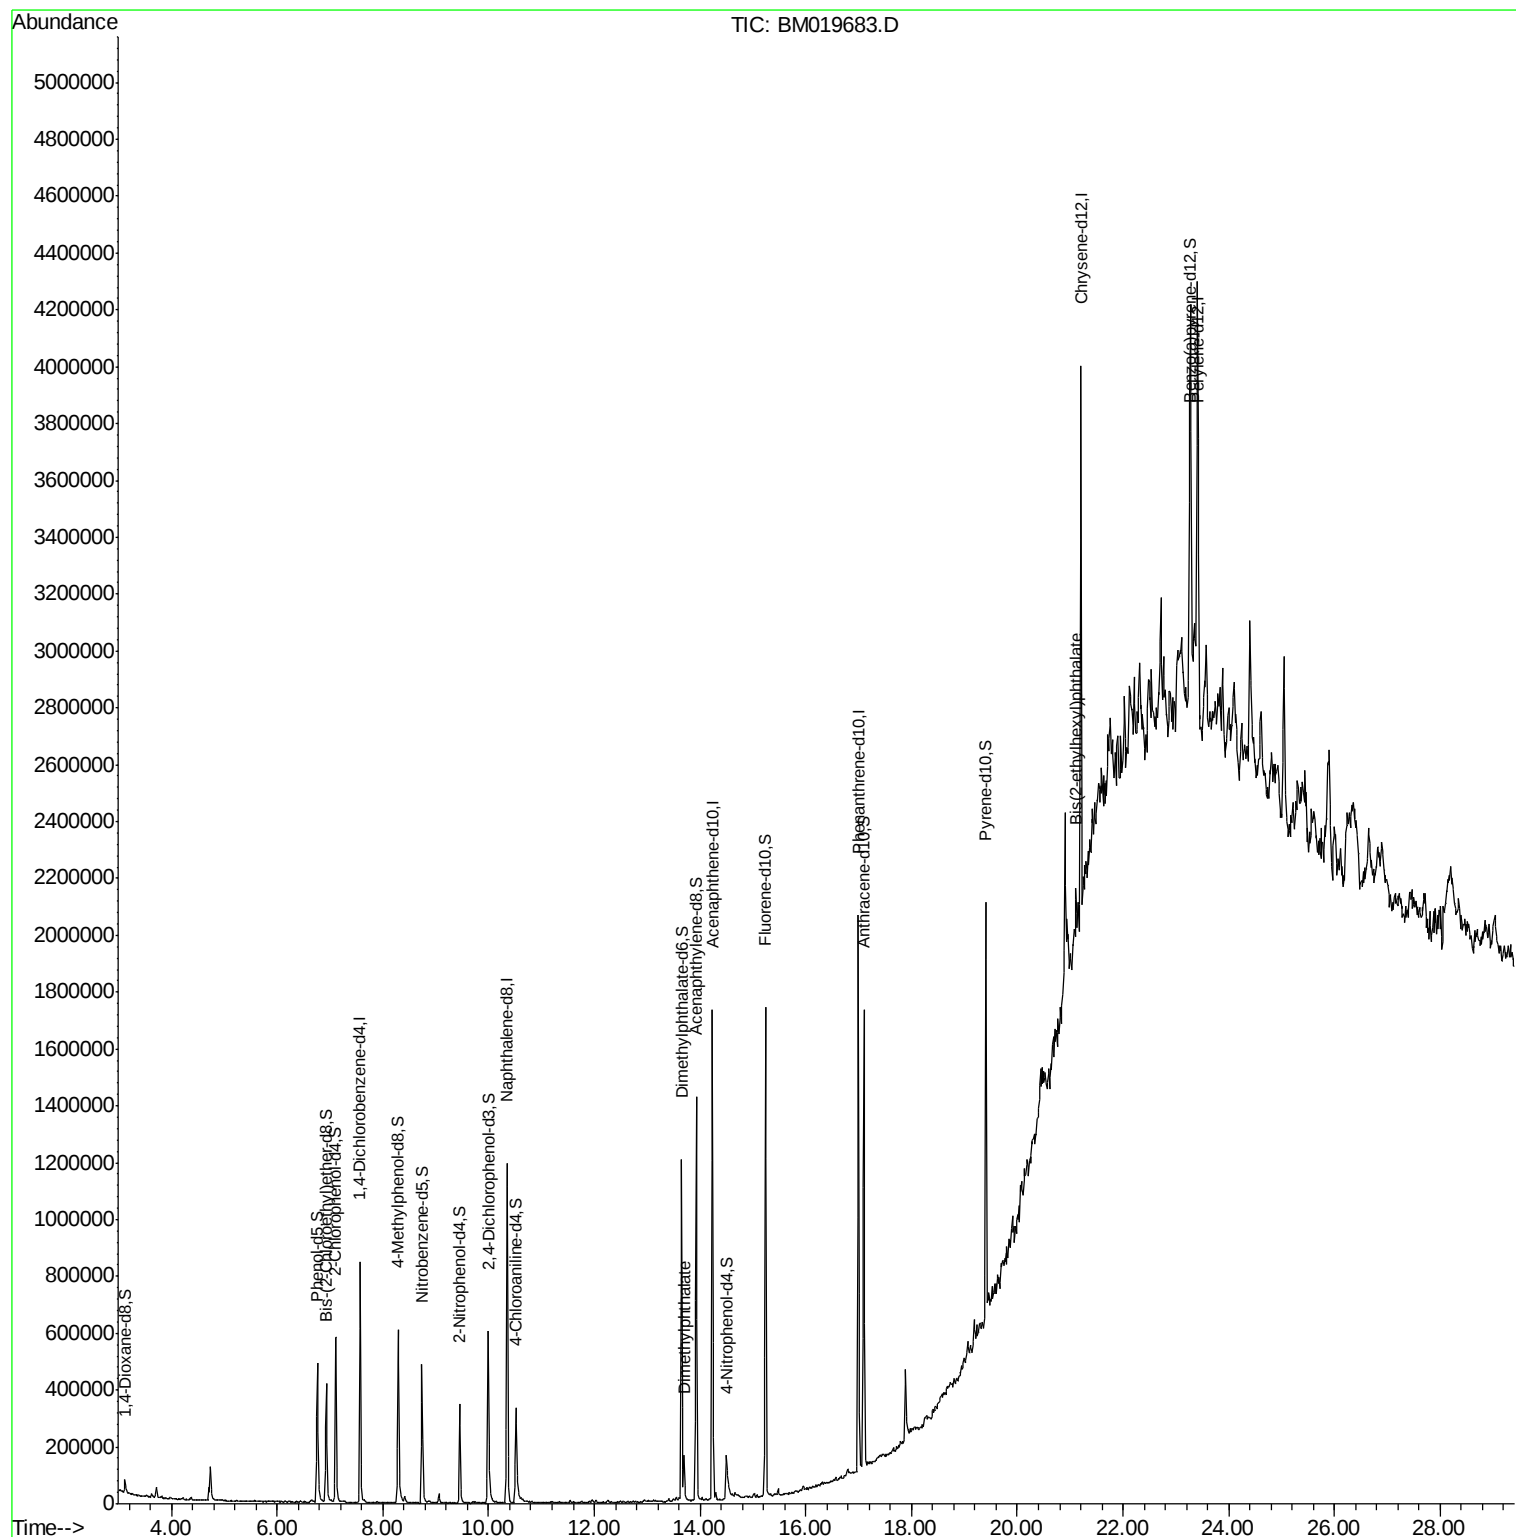


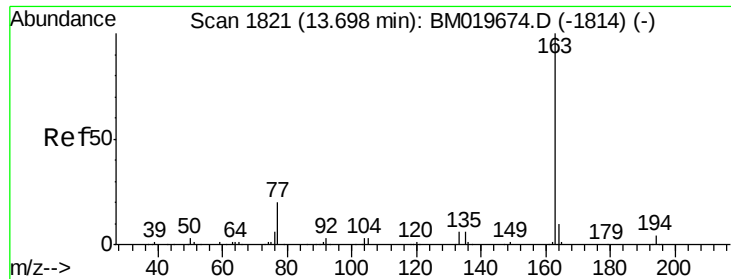




#45
 Dimethylphthalate
 Concen: 2.329 ng/ul
 RT: 13.70 min Scan# 1822
 Delta R.T. -0.02 min
 Lab File: BM019683.D
 Acq: 02 Apr 2019 08:10

Instrument :
 BNA_M
 ClientSampleId :
 BF5J9

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.0	4.0	6.0
164	9.2	8.4	12.6

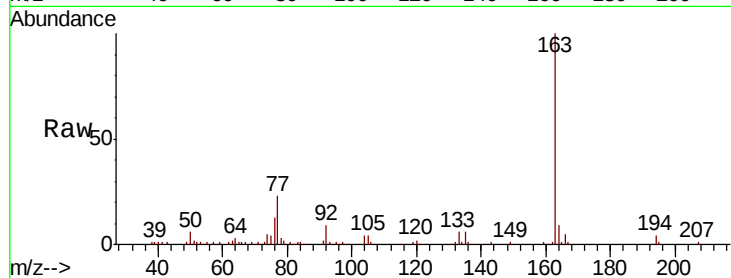


Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

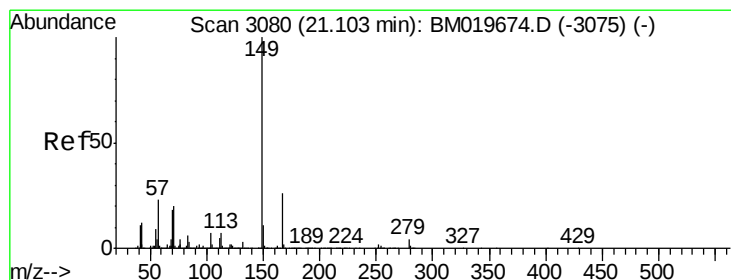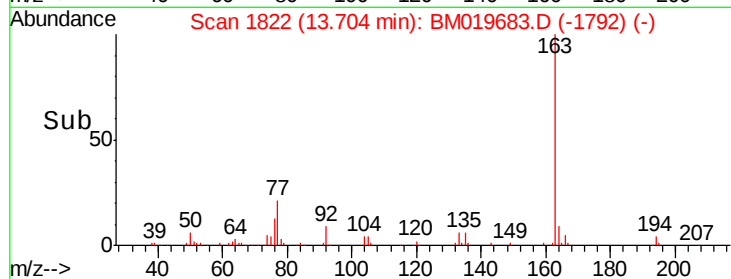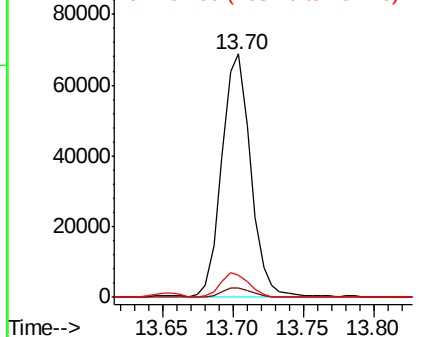

#84
 Bis(2-ethylhexyl)phthalate
 Concen: 2.001 ng/ul
 RT: 21.11 min Scan# 3081
 Delta R.T. -0.02 min
 Lab File: BM019683.D
 Acq: 02 Apr 2019 08:10

Tgt Ion	Ratio	Lower	Upper
149	100		
167	32.0	23.0	34.6
279	7.9	4.3	6.5#

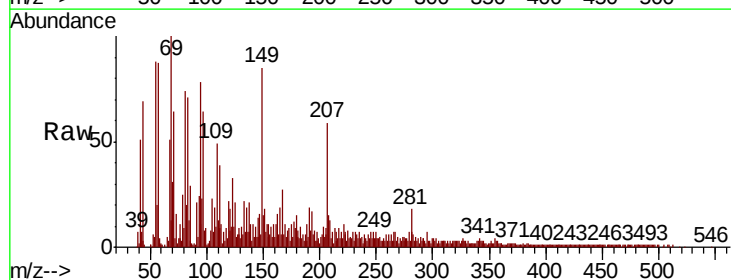

Abundance Ion 149.00 (148.70 to 149.70): E
 Ion 167.00 (166.70 to 167.70): E
 Ion 279.00 (278.70 to 279.70): E

