

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM040119\
 Data File : BM019686.D
 Acq On : 02 Apr 2019 10:00
 Operator : JU/SJ
 Sample : K2119-13
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF5A8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.122	20	23	30	rVB	58037	78329	2.97%	0.207%
2	3.534	90	93	97	rVB3	9337	10657	0.40%	0.028%
3	3.628	105	109	117	rVB	37708	53109	2.02%	0.141%
4	3.716	121	124	129	rVB	21590	36435	1.38%	0.096%
5	3.822	136	142	148	rVB6	8666	17314	0.66%	0.046%
6	4.369	232	235	244	rVB4	9323	14014	0.53%	0.037%
7	4.563	265	268	269	rBV3	2618	2721	0.10%	0.007%
8	4.716	290	294	297	rBV	20005	27844	1.06%	0.074%
9	4.751	297	300	310	rVB	18816	31036	1.18%	0.082%
10	5.240	381	383	386	rVB5	3343	3614	0.14%	0.010%
11	5.387	406	408	412	rBV3	2191	2828	0.11%	0.007%
12	6.657	620	624	627	rVB4	1770	2954	0.11%	0.008%
13	6.763	636	642	662	rBV	587025	1138088	43.21%	3.011%
14	6.928	664	670	689	rVV	508054	864892	32.84%	2.288%
15	7.110	694	701	716	rVB	704640	1148244	43.60%	3.038%
16	7.575	772	780	787	rBV	884153	1394837	52.96%	3.691%
17	7.634	787	790	799	rVB5	12504	26120	0.99%	0.069%
18	7.887	830	833	836	rBV5	3091	3876	0.15%	0.010%
19	8.292	895	902	919	rBV	648513	1152003	43.74%	3.048%
20	8.416	919	923	929	rVB2	15915	26981	1.02%	0.071%
21	8.745	972	979	994	rBV	576311	1016894	38.61%	2.691%
22	8.863	994	999	1001	rVV5	6222	10914	0.41%	0.029%
23	8.892	1001	1004	1007	rVB4	4670	6358	0.24%	0.017%
24	9.063	1029	1033	1038	rVB	17585	24628	0.94%	0.065%
25	9.457	1093	1100	1117	rBV	425197	755481	28.69%	1.999%
26	9.734	1139	1147	1156	rBV7	9553	33061	1.26%	0.087%
27	9.986	1184	1190	1212	rBV	683666	1287040	48.87%	3.405%
28	10.351	1245	1252	1260	rBV	1193491	1981418	75.23%	5.243%
29	10.516	1271	1280	1299	rBV	523802	1158810	44.00%	3.066%
30	10.980	1354	1359	1364	rVB3	1914	2697	0.10%	0.007%
31	11.180	1388	1393	1402	rBV6	12321	32725	1.24%	0.087%
32	11.345	1419	1421	1424	rVB2	3411	2676	0.10%	0.007%
33	11.469	1438	1442	1445	rBV2	2055	2920	0.11%	0.008%
34	11.545	1453	1455	1460	rVB3	2587	3670	0.14%	0.010%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM040119\
 Data File : BM019686.D
 Acq On : 02 Apr 2019 10:00
 Operator : JU/SJ
 Sample : K2119-13
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF5A8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Title : SVOA CALIBRATION

35	11.763	1486	1492	1494	rBV3	3796	5395	0.20%	0.014%
36	11.957	1521	1525	1534	rVB2	9592	19653	0.75%	0.052%
37	12.527	1616	1622	1626	rBV5	7188	17841	0.68%	0.047%
38	12.580	1629	1631	1636	rVB5	1998	3118	0.12%	0.008%
39	12.727	1650	1656	1660	rBV5	4372	7425	0.28%	0.020%
40	12.810	1669	1670	1675	rVB3	2433	3033	0.12%	0.008%
41	12.933	1688	1691	1695	rBV2	3799	5500	0.21%	0.015%
42	13.022	1701	1706	1711	rBV3	11925	17724	0.67%	0.047%
43	13.110	1713	1721	1727	rBV2	29867	47597	1.81%	0.126%
44	13.192	1733	1735	1739	rVB2	2970	3408	0.13%	0.009%
45	13.516	1785	1790	1794	rVB4	3272	5245	0.20%	0.014%
46	13.604	1802	1805	1807	rBV3	2380	3582	0.14%	0.009%
47	13.651	1807	1813	1818	rVV	1276367	1819029	69.07%	4.813%
48	13.704	1818	1822	1838	rVB	533708	766562	29.11%	2.028%
49	13.886	1850	1853	1854	rBV	5238	5452	0.21%	0.014%
50	13.927	1854	1860	1870	rVB	1545169	2194563	83.33%	5.807%
51	14.039	1877	1879	1883	rVB2	2241	2833	0.11%	0.007%
52	14.116	1888	1892	1897	rVB	13290	16614	0.63%	0.044%
53	14.233	1906	1912	1921	rBV2	1450907	2250453	85.45%	5.954%
54	14.498	1951	1957	1974	rBV	170621	490293	18.62%	1.297%
55	14.663	1981	1985	1996	rVB2	68488	112815	4.28%	0.298%
56	14.804	2006	2009	2012	rVB3	3072	4444	0.17%	0.012%
57	15.021	2041	2046	2051	rBV	7064	12162	0.46%	0.032%
58	15.074	2051	2055	2060	rVV2	14091	17475	0.66%	0.046%
59	15.239	2076	2083	2094	rBV	1787076	2610660	99.13%	6.907%
60	15.316	2094	2096	2100	rVB5	3455	4450	0.17%	0.012%
61	15.404	2106	2111	2117	rVV3	17801	26976	1.02%	0.071%
62	15.474	2119	2123	2128	rVV2	20685	31346	1.19%	0.083%
63	15.615	2144	2147	2148	rBV3	3802	3317	0.13%	0.009%
64	15.786	2172	2176	2177	rBV4	4466	6050	0.23%	0.016%
65	15.945	2198	2203	2209	rBV5	11046	25303	0.96%	0.067%
66	16.021	2214	2216	2219	rVB2	5249	5316	0.20%	0.014%
67	16.133	2231	2235	2238	rBV5	4381	5731	0.22%	0.015%
68	16.192	2242	2245	2247	rBV4	3897	4546	0.17%	0.012%
69	16.274	2257	2259	2262	rBV3	4336	6082	0.23%	0.016%
70	16.310	2262	2265	2268	rVB4	5400	7167	0.27%	0.019%
71	16.398	2277	2280	2286	rVB3	8989	12103	0.46%	0.032%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM040119\
 Data File : BM019686.D
 Acq On : 02 Apr 2019 10:00
 Operator : JU/SJ
 Sample : K2119-13
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF5A8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Title : SVOA CALIBRATION

72	16.515	2297	2300	2301	rBV2	4406	4704	0.18%	0.012%
73	16.539	2301	2304	2307	rVB2	11558	14997	0.57%	0.040%
74	16.739	2333	2338	2340	rBV3	15136	20721	0.79%	0.055%
75	16.786	2342	2346	2349	rVB6	10593	16471	0.63%	0.044%
76	16.904	2363	2366	2369	rVB4	4136	4827	0.18%	0.013%
77	16.998	2375	2382	2388	rBV2	1583797	2216888	84.17%	5.866%
78	17.092	2392	2398	2409	rVV2	1581520	2286521	86.82%	6.050%
79	17.274	2426	2429	2430	rBV3	7990	9455	0.36%	0.025%
80	17.315	2432	2436	2439	rVV5	14079	26116	0.99%	0.069%
81	17.374	2442	2446	2451	rVV6	16954	34347	1.30%	0.091%
82	17.474	2460	2463	2469	rVB3	16240	20318	0.77%	0.054%
83	17.657	2490	2494	2499	rVB6	34483	40589	1.54%	0.107%
84	17.886	2528	2533	2537	rBV2	98910	153992	5.85%	0.407%
85	17.968	2544	2547	2553	rVB	14262	21625	0.82%	0.057%
86	18.168	2578	2581	2585	rBV2	23605	29192	1.11%	0.077%
87	18.721	2672	2675	2677	rBV4	15507	21683	0.82%	0.057%
88	18.809	2687	2690	2693	rBV4	34228	38224	1.45%	0.101%
89	19.403	2786	2791	2796	rBV2	1621919	2212970	84.03%	5.855%
90	20.903	3043	3046	3050	rBV2	188772	221569	8.41%	0.586%
91	21.203	3093	3097	3103	rBV	1831000	2360011	89.61%	6.244%
92	23.268	3443	3448	3455	rVB2	1293212	2633669	100.00%	6.968%
93	23.415	3468	3473	3483	rVB2	1331340	2469244	93.76%	6.533%


Sum of corrected areas: 37794584

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM040119\
Data File : BM019686.D
Acq On : 02 Apr 2019 10:00
Operator : JU/SJ
Sample : K2119-13
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF5A8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

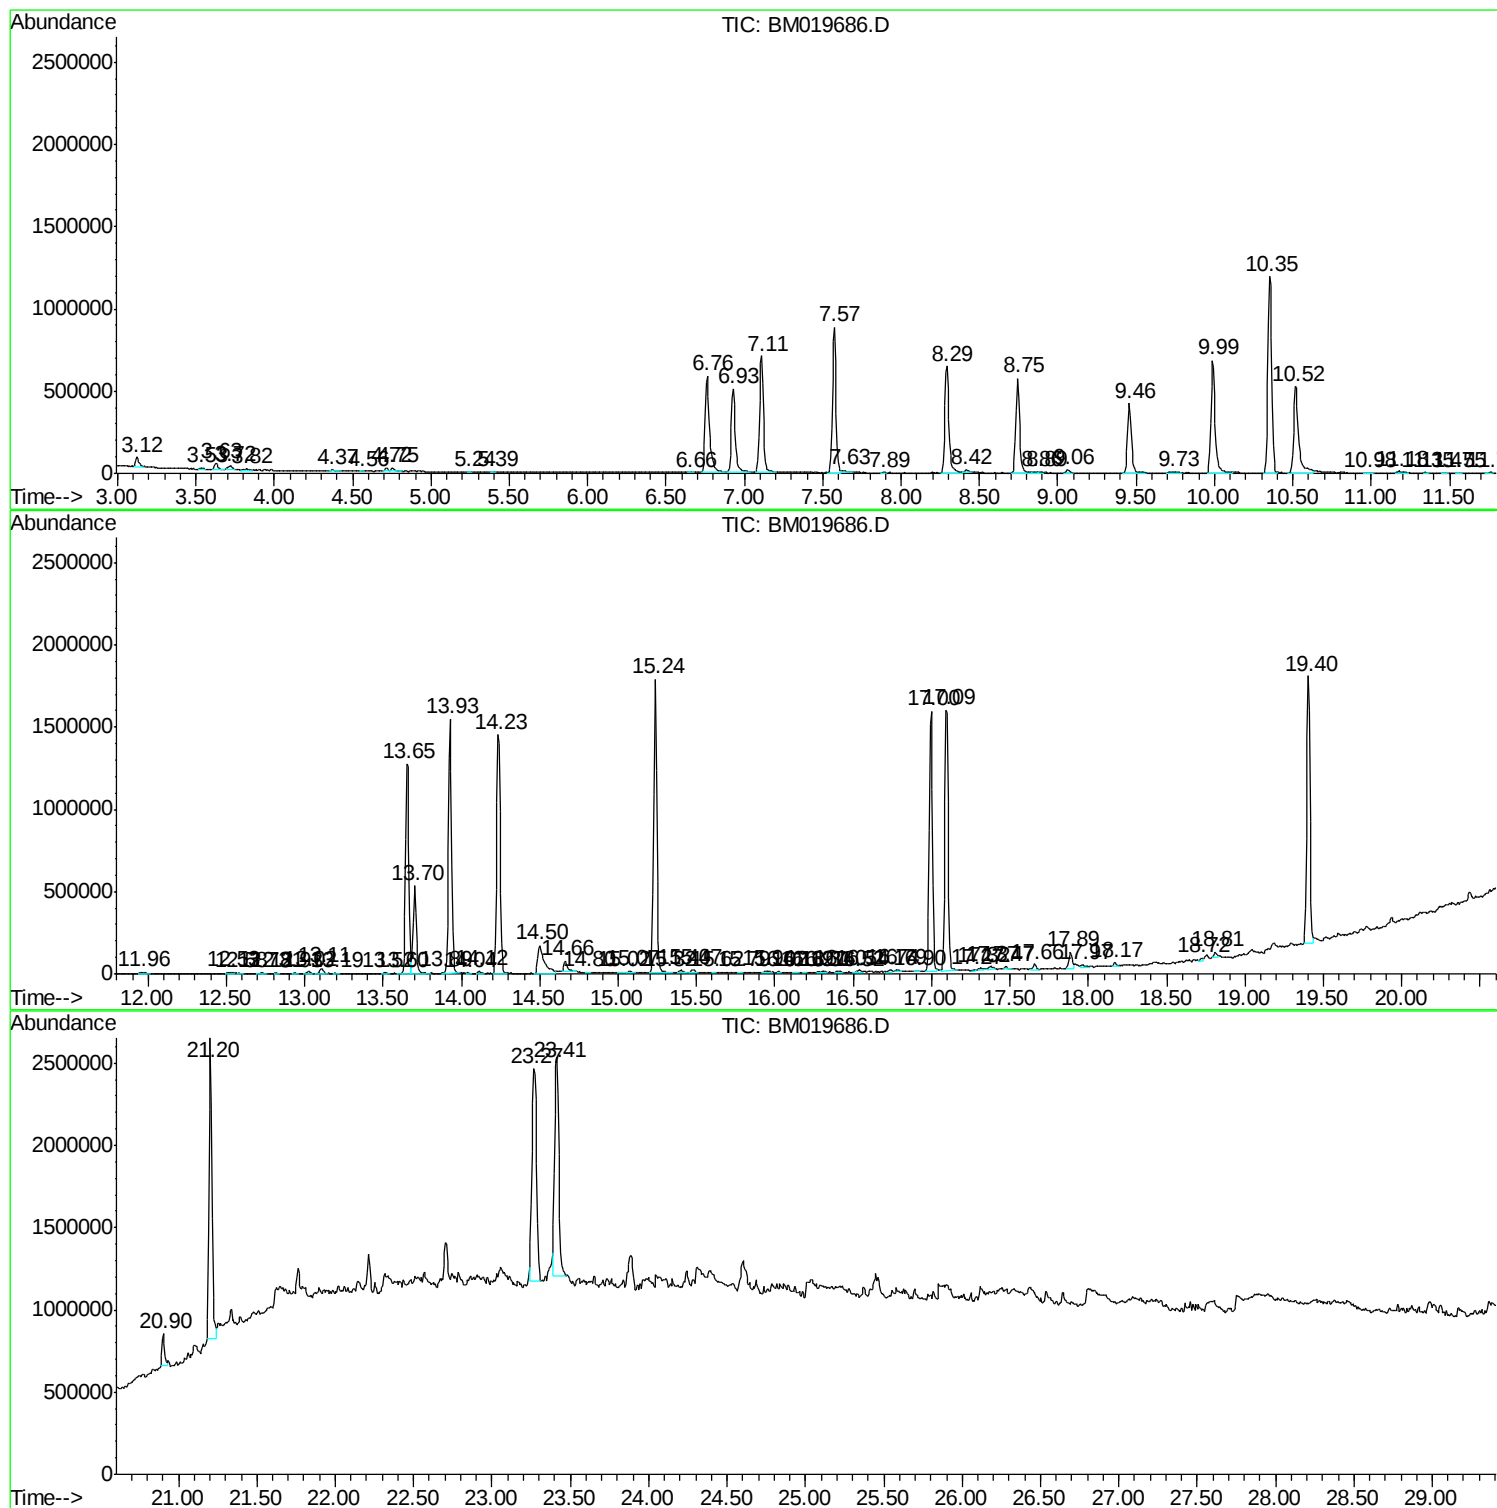

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040119\
Data File : BM019686.D
Acq On : 02 Apr 2019 10:00
Operator : JU/SJ
Sample : K2119-13
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF5A8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040119\
Data File : BM019686.D
Acq On : 02 Apr 2019 10:00
Operator : JU/SJ
Sample : K2119-13
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF5A8

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc