

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM040120\
 Data File : BM025873.D
 Acq On : 31 Mar 2020 19:52
 Operator : CG/JU
 Sample : L2062-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F3E01

Quant Time: Apr 01 01:30:38 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 31 17:29:06 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	142784	20.00	ng/ul	0.00
18) Naphthalene-d8	10.32	136	584258	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.20	164	351108	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.95	188	766847	20.00	ng/ul	0.00
78) Chrysene-d12	21.14	240	839905	20.00	ng/ul	0.00
86) Perylene-d12	23.29	264	997254	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.13	96	20219	5.94	ng/uL	0.00
5) Phenol-d5	6.75	99	342762	30.42	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.90	67	209455	32.56	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	294811	32.23	ng/ul	0.00
13) 4-Methylphenol-d8	8.26	113	272312	29.41	ng/ul	0.00
19) Nitrobenzene-d5	8.70	128	146602	33.76	ng/ul	0.00
22) 2-Nitrophenol-d4	9.42	143	148701	32.21	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.95	165	291597	30.89	ng/ul	0.00
29) 4-Chloroaniline-d4	10.46	131	123713	11.29	ng/ul	0.00
44) Dimethylphthalate-d6	13.62	166	862701	32.33	ng/ul	0.00
47) Acenaphthylene-d8	13.89	160	1065533	33.33	ng/ul	0.00
52) 4-Nitrophenol-d4	14.40	143	108413	21.34	ng/ul	0.00
58) Fluorene-d10	15.20	176	802049	34.24	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.32	200	100590	21.50	ng/ul	0.00
71) Anthracene-d10	17.05	188	1227628	34.27	ng/ul	0.00
79) Pyrene-d10	19.34	212	1342136	33.27	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.16	264	1707106	33.44	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	13.66	163	228613	8.230	ng/ul 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM040120\
Data File : BM025873.D
Acq On : 31 Mar 2020 19:52
Operator : CG/JU
Sample : L2062-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F3E01

Quant Time: Apr 01 01:30:38 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 31 17:29:06 2020
Response via : Initial Calibration

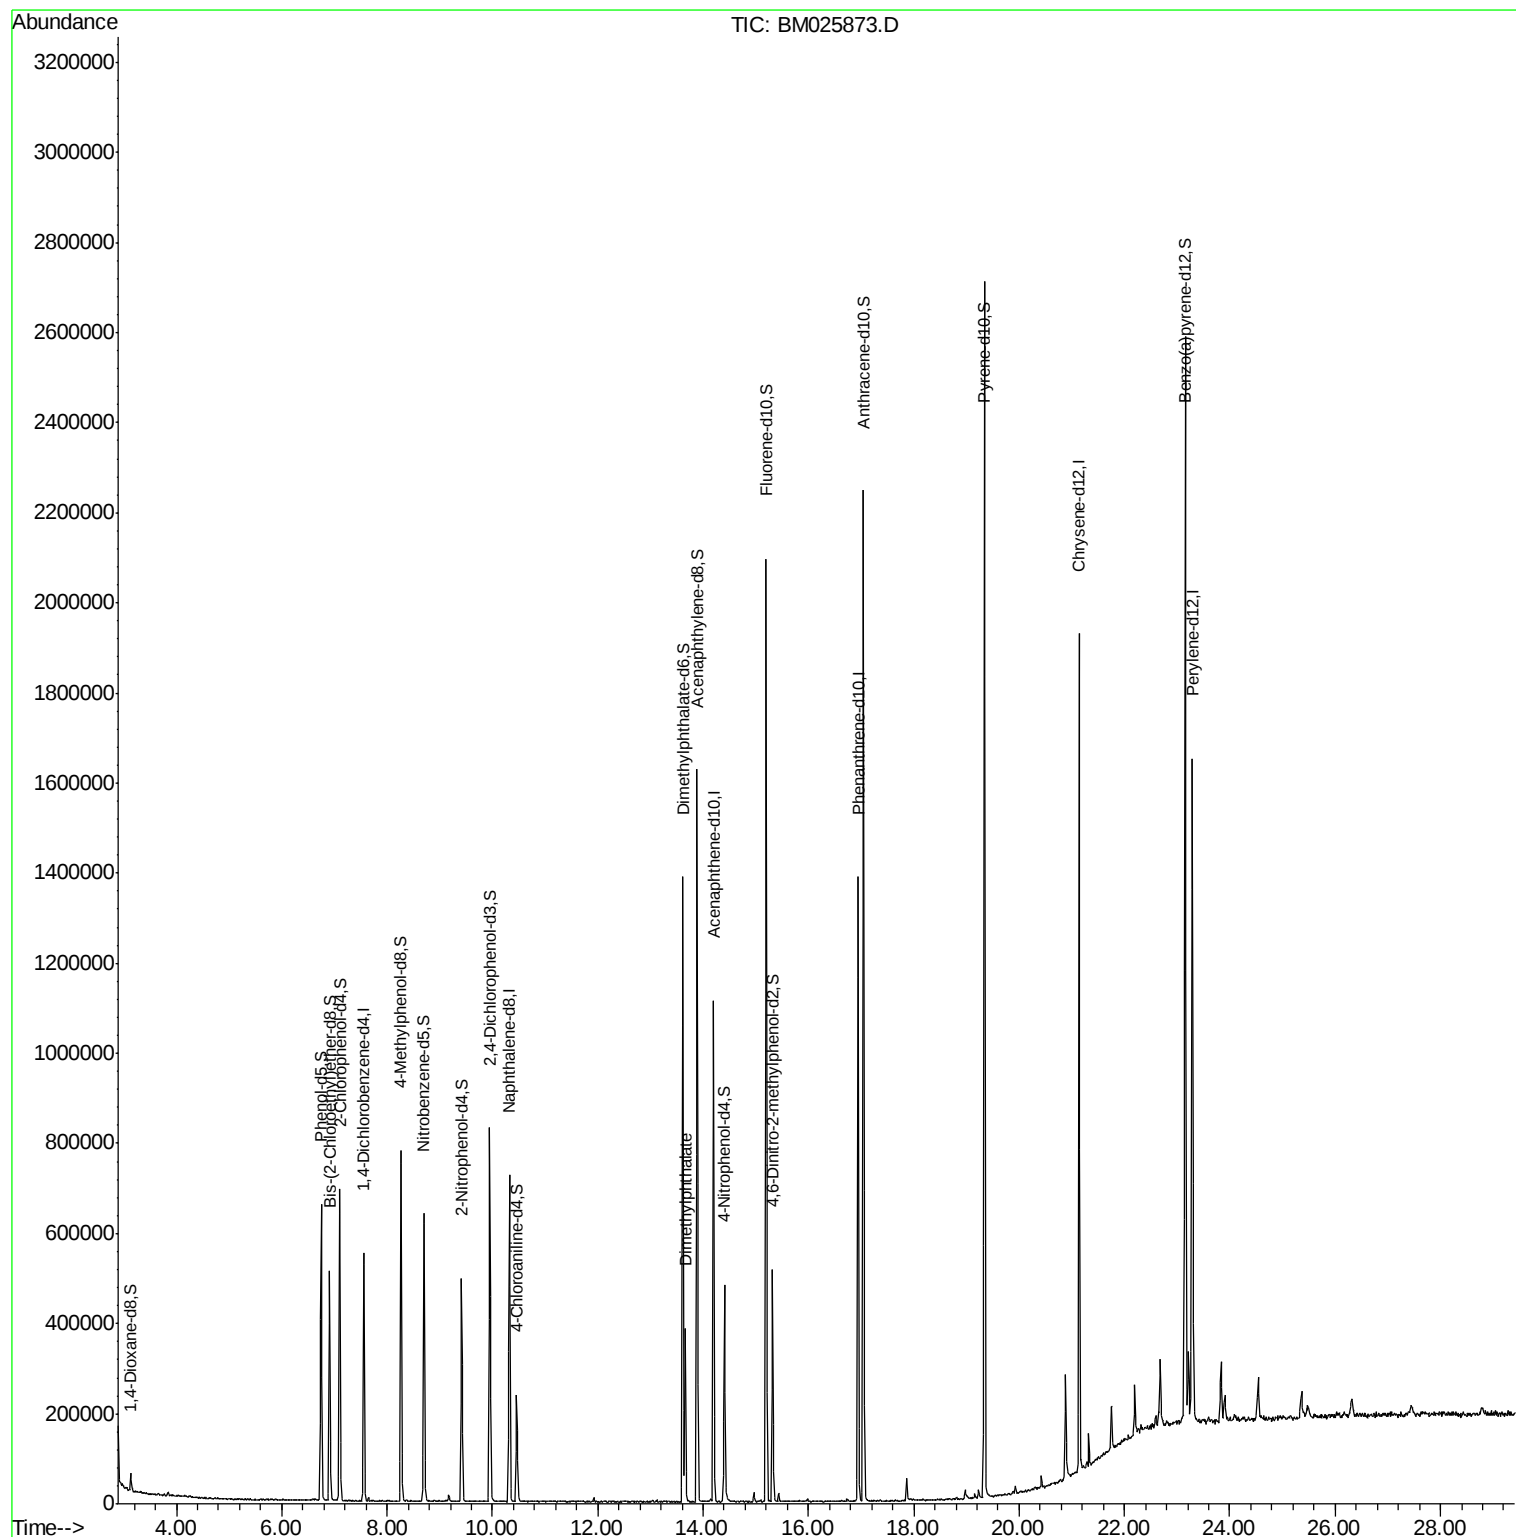

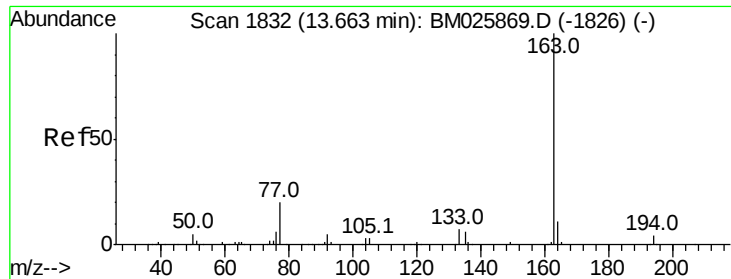

#45

Dimethylphthalate

Concen: 8.230 ng/ul

RT: 13.66 min Scan# 1832

Delta R.T. -0.00 min

Lab File: BM025873.D

Acq: 31 Mar 2020 19:52

Instrument :

BNA_M

ClientSampleId :

F3E01


Tot Ion:163 Resp: 228613

Ion Ratio Lower Upper

163 100

194 4.4 3.5 5.3

164 10.4 8.2 12.4

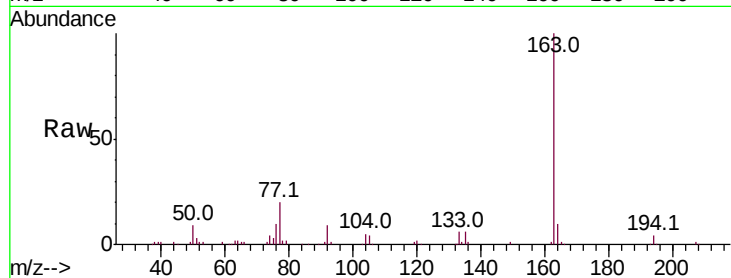

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

