

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM040120\
 Data File : BM025874.D
 Acq On : 31 Mar 2020 20:28
 Operator : CG/JU
 Sample : L2062-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F3E02

Quant Time: Apr 01 01:35:04 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 01 01:28:55 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	147767	20.00	ng/ul	0.00
18) Naphthalene-d8	10.32	136	604125	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.20	164	358850	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.94	188	777248	20.00	ng/ul	0.00
78) Chrysene-d12	21.14	240	844504	20.00	ng/ul	0.00
86) Perylene-d12	23.29	264	957954	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.13	96	26649	7.57	ng/uL	0.00
5) Phenol-d5	6.75	99	437311	37.50	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.90	67	264417	39.72	ng/ul	0.00
9) 2-Chlorophenol-d4	7.10	132	375906	39.72	ng/ul	0.00
13) 4-Methylphenol-d8	8.26	113	352352	36.77	ng/ul	0.00
19) Nitrobenzene-d5	8.70	128	186329	41.50	ng/ul	0.00
22) 2-Nitrophenol-d4	9.42	143	196514	41.17	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.95	165	364730	37.36	ng/ul	0.00
29) 4-Chloroaniline-d4	10.46	131	286854	25.31	ng/ul	0.00
44) Dimethylphthalate-d6	13.62	166	1106149	40.56	ng/ul	0.00
47) Acenaphthylene-d8	13.89	160	1370780	41.95	ng/ul	0.00
52) 4-Nitrophenol-d4	14.40	143	154145	29.69	ng/ul	0.00
58) Fluorene-d10	15.20	176	1003528	41.92	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.32	200	137496	28.99	ng/ul	0.00
71) Anthracene-d10	17.04	188	1523562	41.97	ng/ul	0.00
79) Pyrene-d10	19.34	212	1649226	40.66	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.15	264	2030484	41.40	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.66	163	198577	6.995	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM040120\
Data File : BM025874.D
Acq On : 31 Mar 2020 20:28
Operator : CG/JU
Sample : L2062-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F3E02

Quant Time: Apr 01 01:35:04 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031420MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 01 01:28:55 2020
Response via : Initial Calibration

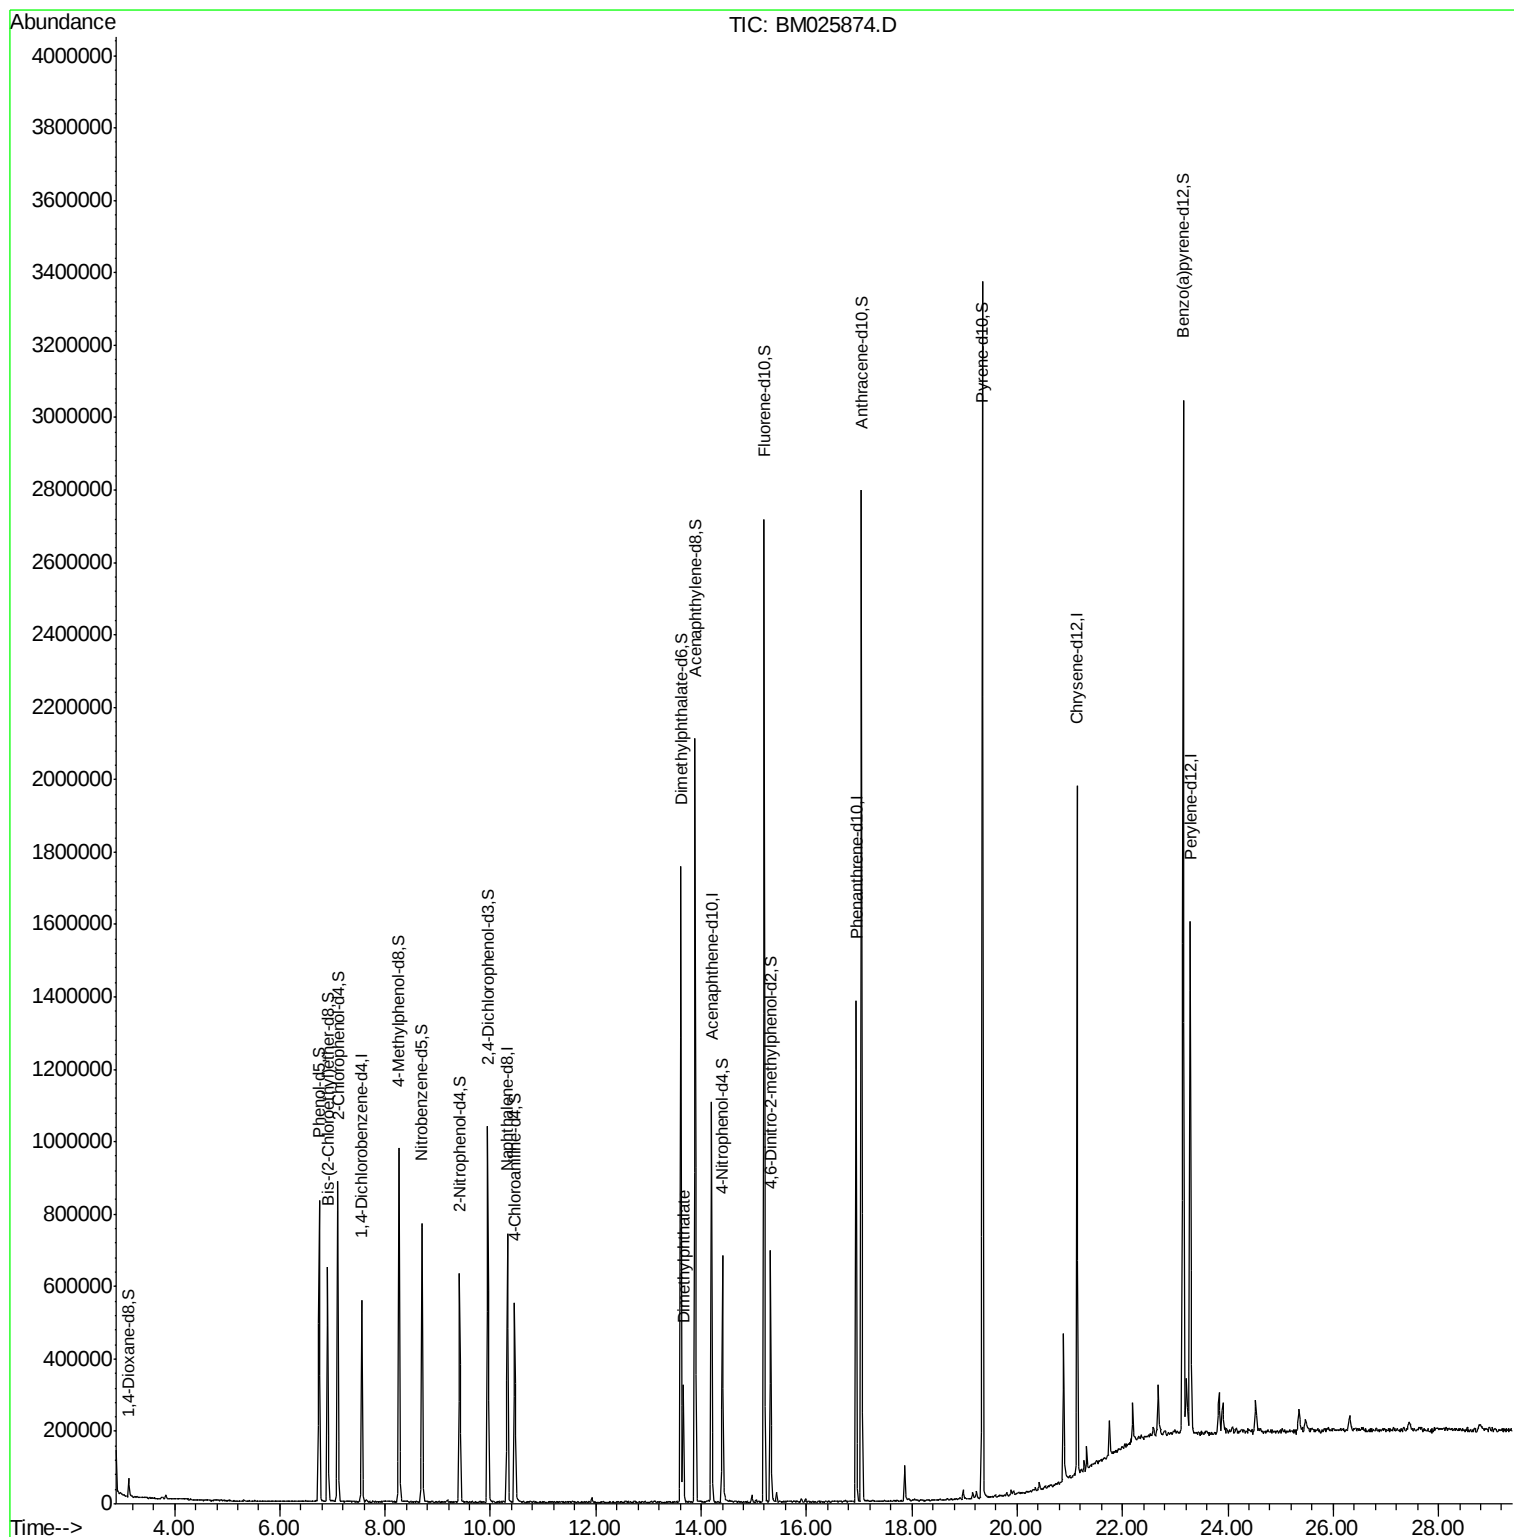

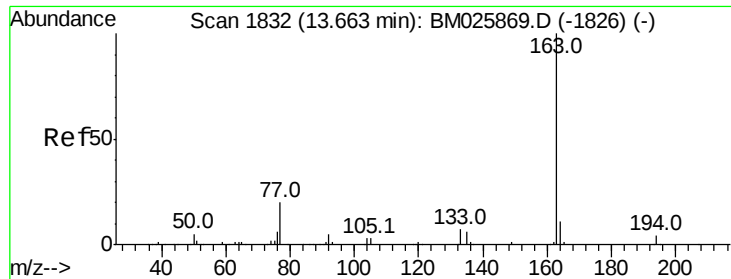

#45

Dimethylphthalate

Concen: 6.995 ng/ul

RT: 13.66 min Scan# 1832

Delta R.T. -0.00 min

Lab File: BM025874.D

Acq: 31 Mar 2020 20:28

Instrument :

BNA_M

ClientSampleId :

F3E02


Tot Ion:163 Resp: 198577

Ion Ratio Lower Upper

163 100

194 4.3 3.5 5.3

164 10.8 8.2 12.4

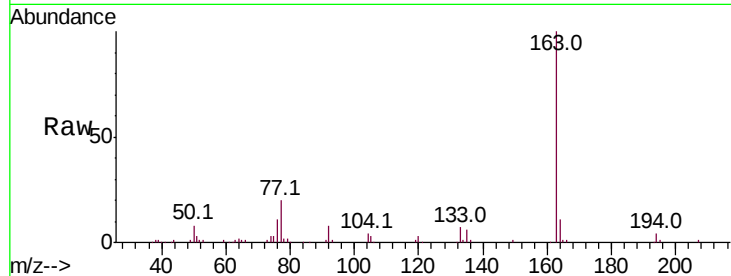

Abundance Ion 163.00 (162.70 to 163.70): E

200000 Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

