


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040121\
 Data File : BM029300.D
 Acq On : 01 Apr 2021 11:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 01 16:52:48 2021

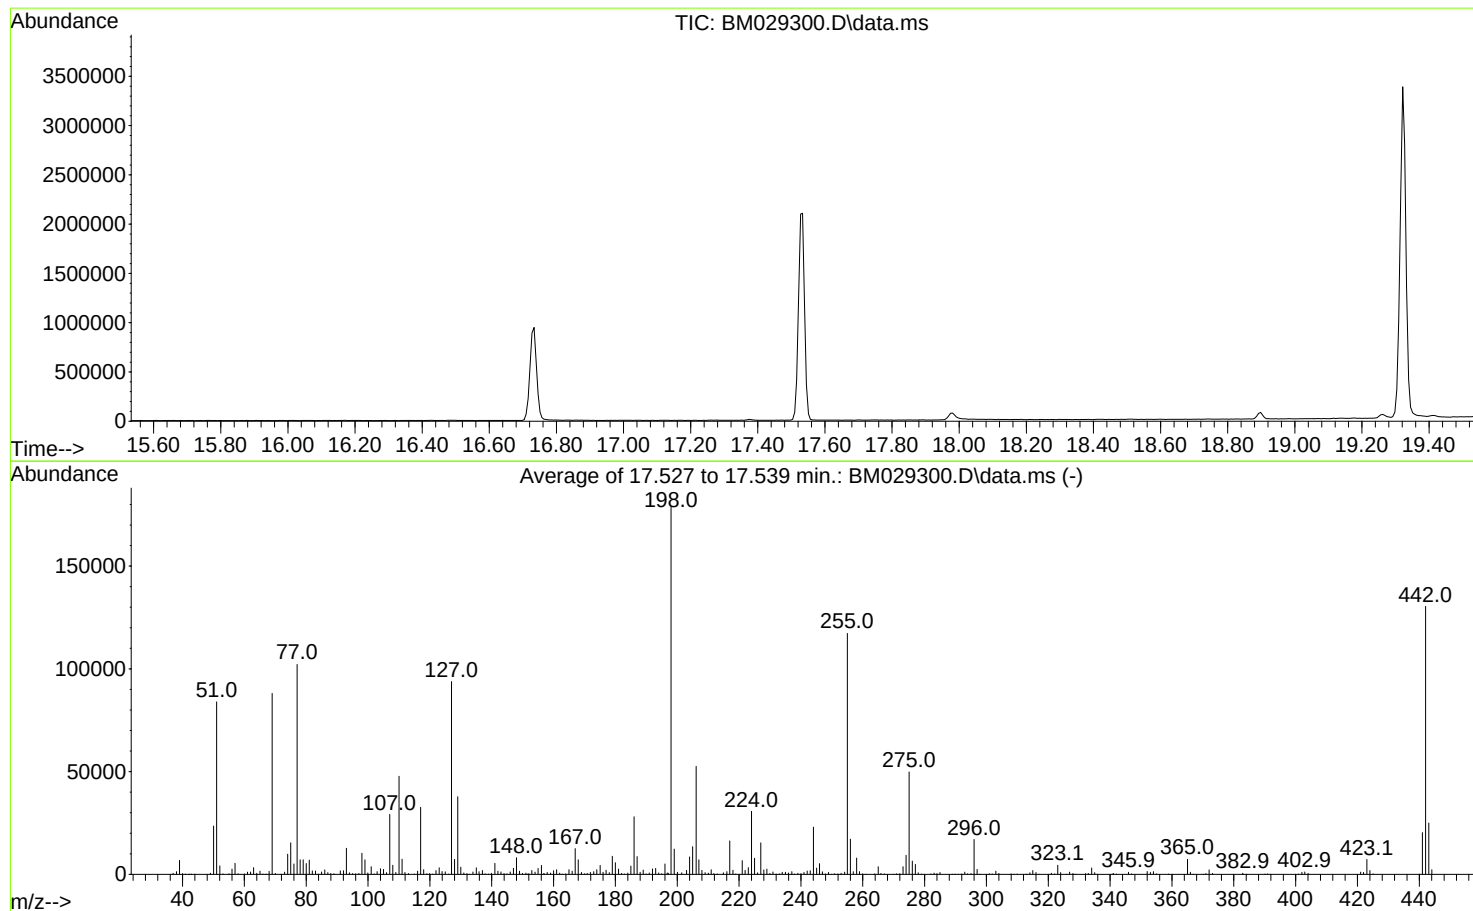

AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.9	83935	PASS
68	69	0.00	2	1.7	1479	PASS
69	198	0.00	100	49.2	88065	PASS
70	69	0.00	2	0.5	466	PASS
127	198	10	80	52.4	93797	PASS
197	198	0.00	2	0.4	699	PASS
198	198	100	100	100.0	179005	PASS
199	198	5	9	6.9	12308	PASS
275	198	10	60	27.9	49856	PASS
365	198	1	100	4.1	7350	PASS
441	198	0.01	100	11.3	20301	PASS
442	442	50	100	100.0	130400	PASS
443	442	15	24	19.2	24997	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/1/2021	BNA_M	<u>BM029300.D</u>
Compound Name	Response	Retention Time
DDT	731593	20.55
DDD	1184	20.12
DDE	738	19.61
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1922	733515	0.26

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040121\
 Data File : BM029300.D
 Acq On : 01 Apr 2021 11:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Apr 01 16:53:53 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 01 16:52:48 2021
 Response via : Initial Calibration

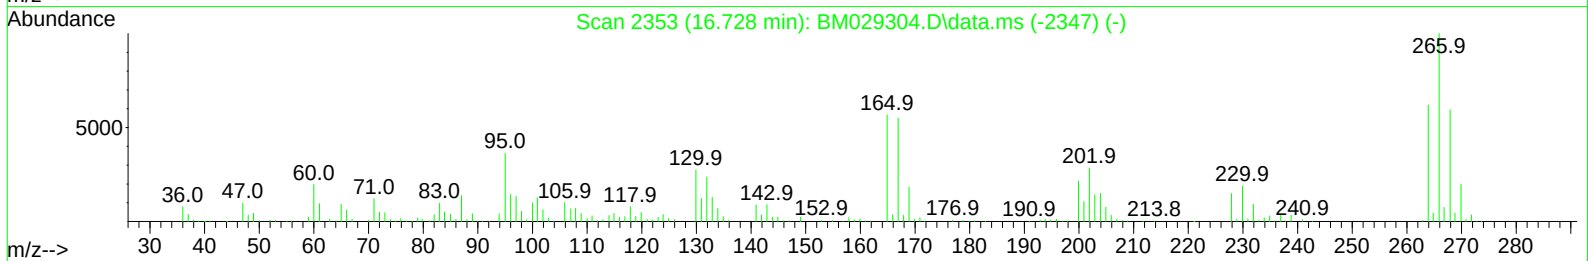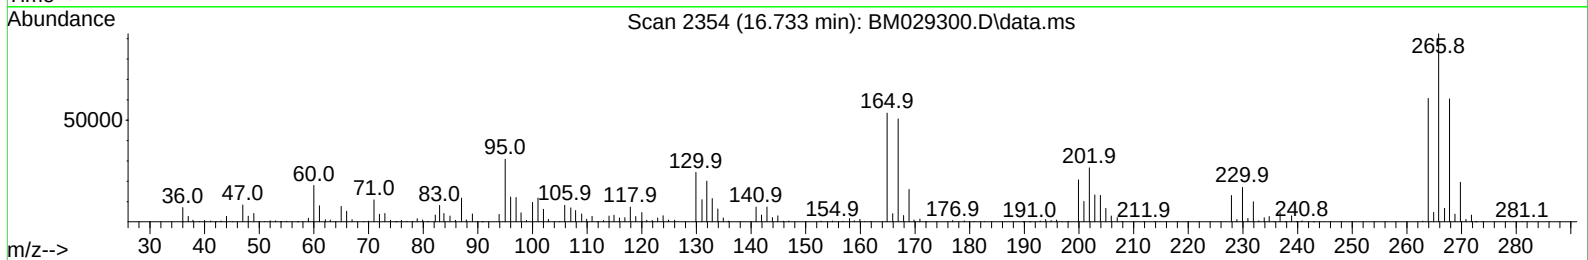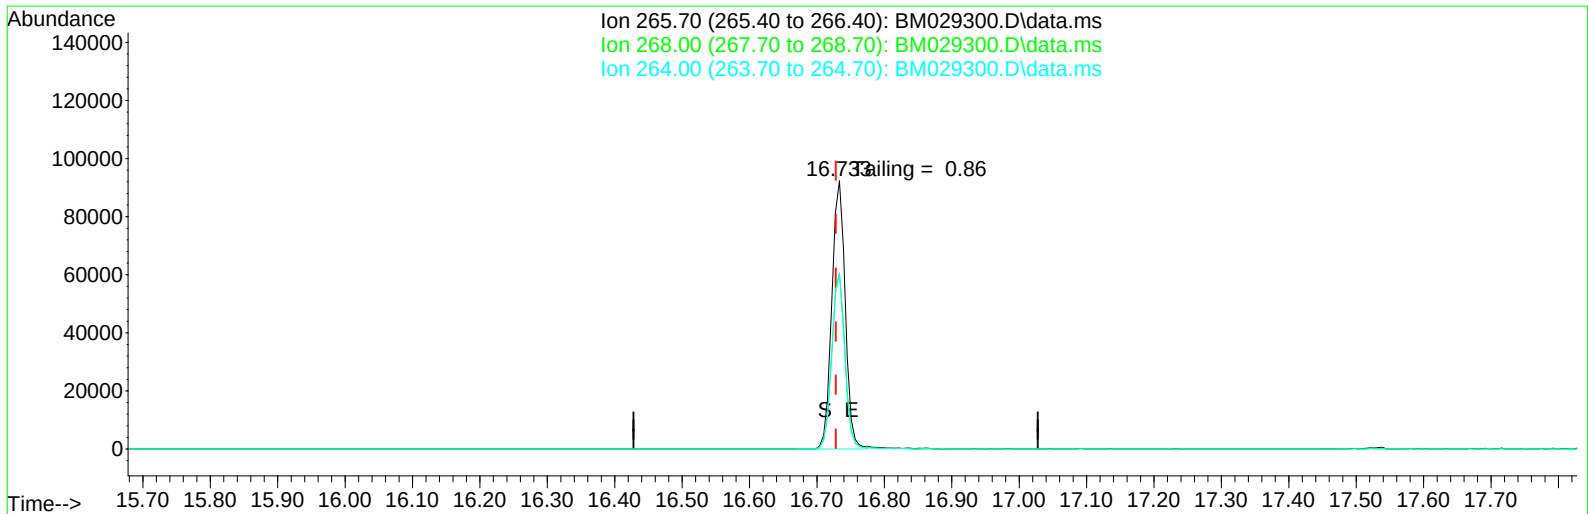

TIC: BM029300.D\data.ms

(70) Pentachlorophenol (C)

16.733min (+ 0.005) 0.00 ng




response 128856

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.20	65.45
264.00	63.60	65.67
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040121\
 Data File : BM029300.D
 Acq On : 01 Apr 2021 11:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Apr 01 16:53:53 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 01 16:52:48 2021
 Response via : Initial Calibration

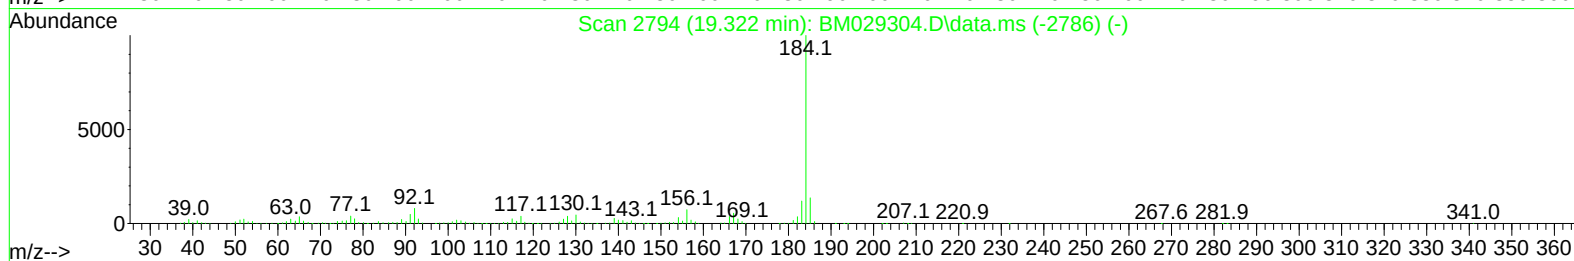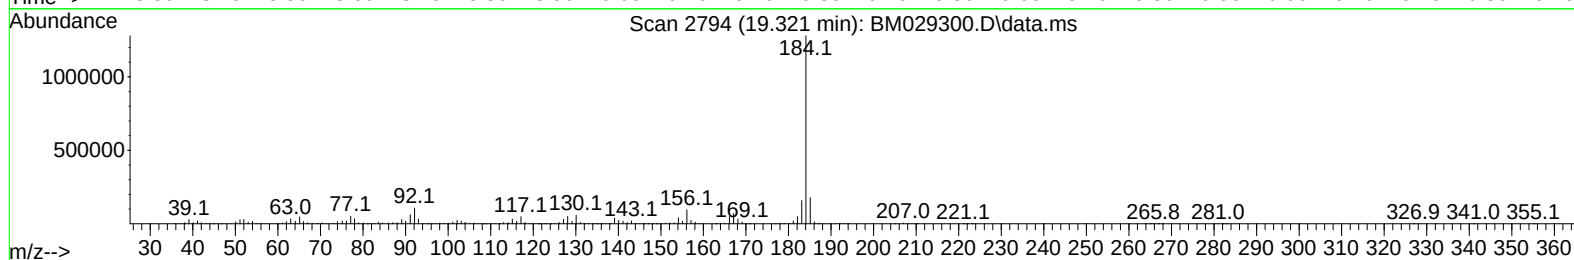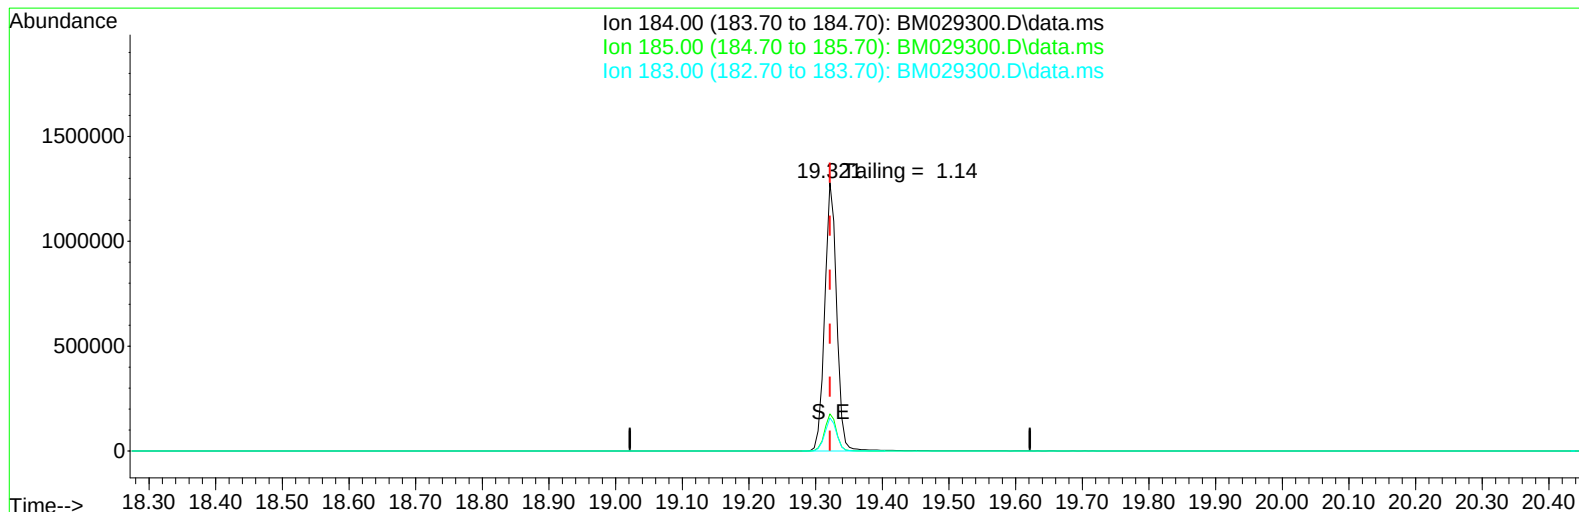

TIC: BM029300.D\data.ms

(77) Benzidine

19.321min (-0.000) 753743.07 ng

response 1589022

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.86
183.00	12.20	12.35
0.00	0.00	0.00