

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040219\
 Data File : BM019696.D
 Acq On : 02 Apr 2019 18:00
 Operator : JU/SJ
 Sample : K2148-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF5F6

Quant Time: Apr 03 01:21:38 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 03 01:13:19 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	130250	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.35	136	587720	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.23	164	353464	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.99	188	839442	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	959889	20.00	ng/ul	0.00
86) Perylene-d12	23.41	264	1040468	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.12	96	25921	7.79	ng/uL	0.00
5) Phenol-d5	6.76	99	295499	25.48	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	197877	25.48	ng/ul	-0.01
9) 2-Chlorophenol-d4	7.10	132	239413	27.23	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	250607	28.78	ng/ul	0.00
19) Nitrobenzene-d5	8.74	128	118179	28.19	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.45	143	139152	29.82	ng/ul	-0.01
26) 2,4-Dichlorophenol-d3	9.99	165	229556	26.07	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	341987	32.35	ng/ul	0.00
44) Dimethylphthalate-d6	13.65	166	913909	32.04	ng/ul	-0.01
47) Acenaphthylene-d8	13.92	160	1075086	30.15	ng/ul	-0.01
52) 4-Nitrophenol-d4	14.49	143	121562	27.19	ng/ul	0.00
58) Fluorene-d10	15.23	176	757902	30.84	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	138026	24.86	ng/ul	0.00
71) Anthracene-d10	17.09	188	1275410	31.66	ng/ul	0.00
79) Pyrene-d10	19.40	212	1405105	31.69	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.27	264	1652524	29.96	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.70	163	169162	5.912	ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040219\
Data File : BM019696.D
Acq On : 02 Apr 2019 18:00
Operator : JU/SJ
Sample : K2148-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF5F6

Quant Time: Apr 03 01:21:38 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 03 01:13:19 2019
Response via : Initial Calibration

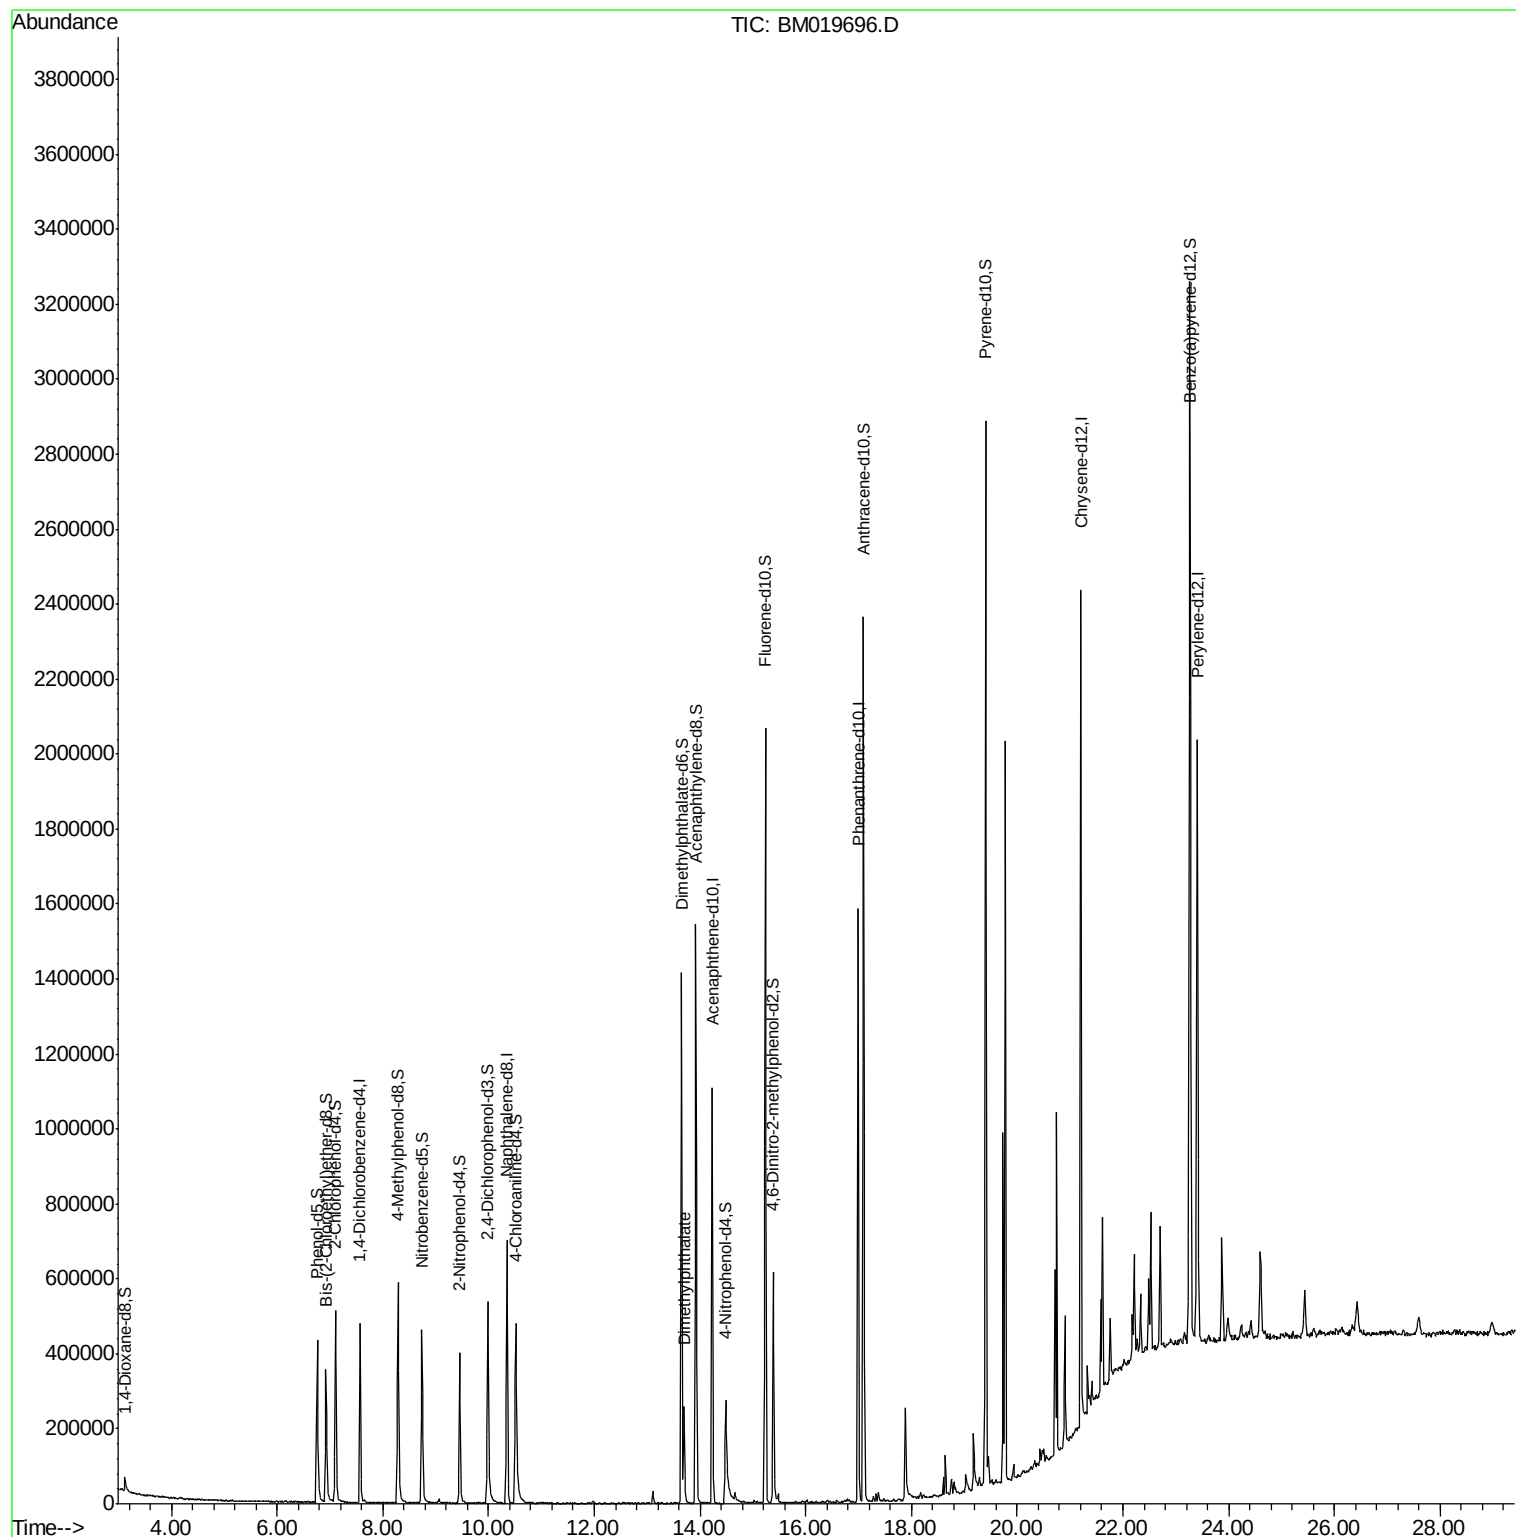


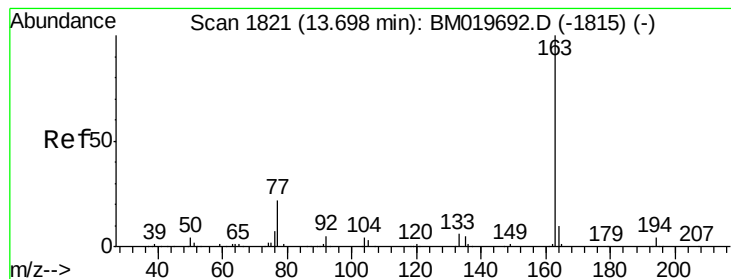

#45
 Dimethylphthalate
 Concen: 5.912 ng/ul
 RT: 13.70 min Scan# 1821
 Delta R.T. -0.01 min
 Lab File: BM019696.D
 Acq: 02 Apr 2019 18:00

Instrument :
 BNA_M
 ClientSampleId :
 BF5F6

Tgt Ion	Ratio	Lower	Upper
163	100		
194	3.3	4.0	6.0#
164	10.4	8.4	12.6

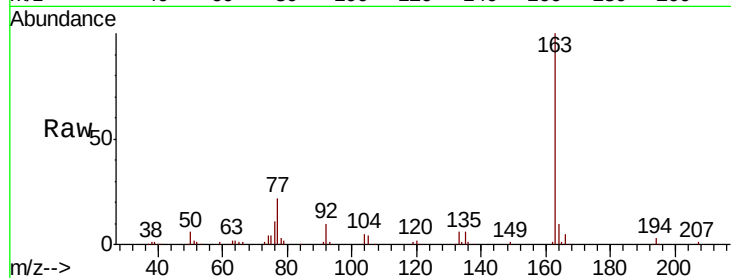

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

