

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040219\
 Data File : BM019713.D
 Acq On : 03 Apr 2019 04:26
 Operator : JU/SJ
 Sample : K2168-09
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF636

Quant Time: Apr 03 05:57:42 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 03 05:54:32 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	152339	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.35	136	717297	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.23	164	432417	20.00	ng/ul	-0.01
62) Phenanthrene-d10	16.99	188	970423	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	993507	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	929742	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.12	96	26071	6.70	ng/uL	0.00
5) Phenol-d5	6.75	99	316519	23.33	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	6.92	67	211908	23.33	ng/ul	-0.01
9) 2-Chlorophenol-d4	7.10	132	256392	24.94	ng/ul	0.00
13) 4-Methylphenol-d8	8.28	113	264124	25.94	ng/ul	-0.01
19) Nitrobenzene-d5	8.74	128	125030	24.44	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.45	143	146794	25.78	ng/ul	-0.01
26) 2,4-Dichlorophenol-d3	9.98	165	246053	22.90	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.51	131	346821	26.88	ng/ul	-0.01
44) Dimethylphthalate-d6	13.65	166	917355	26.29	ng/ul	-0.01
47) Acenaphthylene-d8	13.92	160	1096114	25.12	ng/ul	-0.01
52) 4-Nitrophenol-d4	14.49	143	108647	19.86	ng/ul	0.00
58) Fluorene-d10	15.23	176	759075	25.25	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.38	200	118981	18.54	ng/ul	0.00
71) Anthracene-d10	17.09	188	1206387	25.91	ng/ul	-0.01
79) Pyrene-d10	19.40	212	1293960	28.20	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	1205518	24.46	ng/ul	-0.01


Target Compounds					Qvalue	
45) Dimethylphthalate	13.70	163	122497	3.499	ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040219\
Data File : BM019713.D
Acq On : 03 Apr 2019 04:26
Operator : JU/SJ
Sample : K2168-09
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF636

Quant Time: Apr 03 05:57:42 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 03 05:54:32 2019
Response via : Initial Calibration

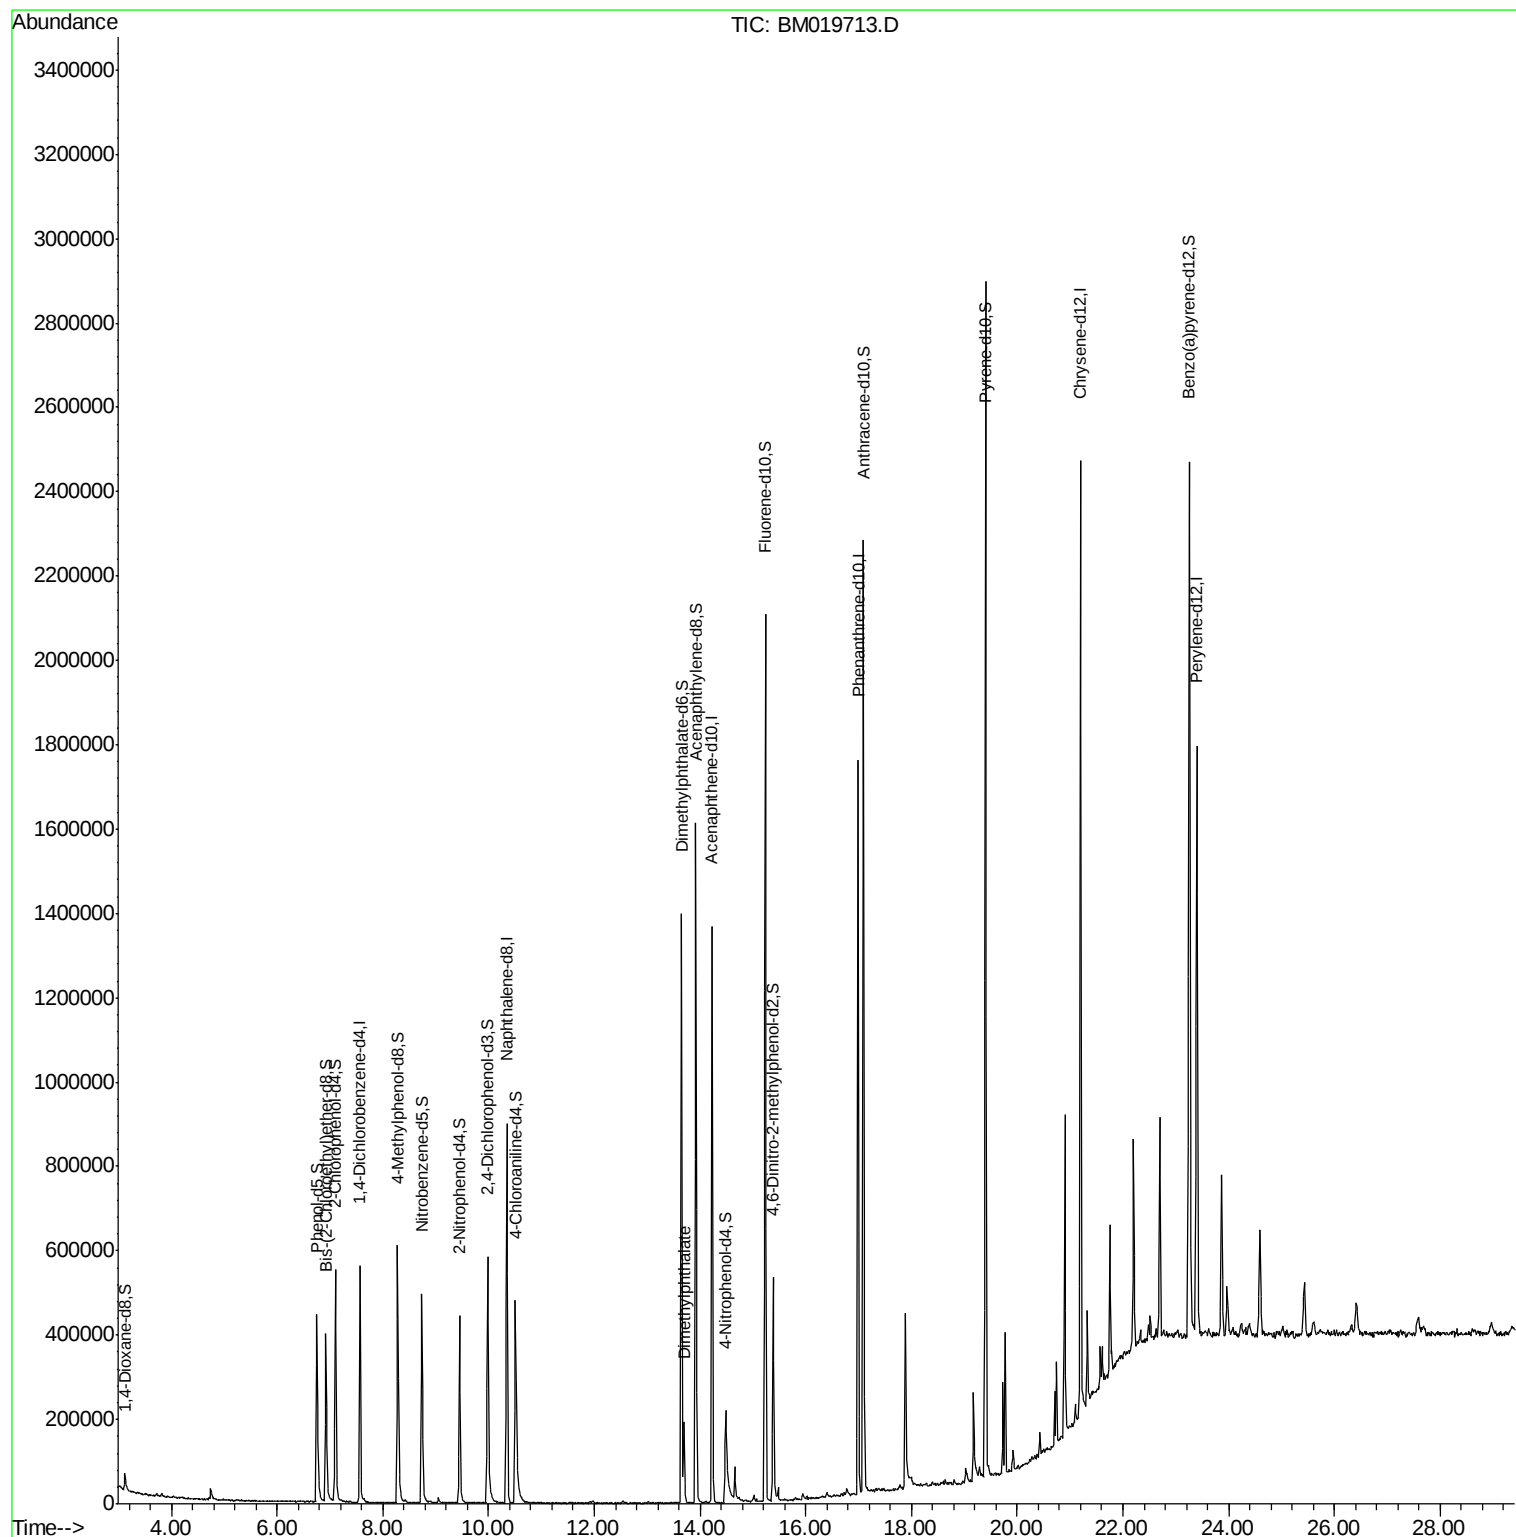

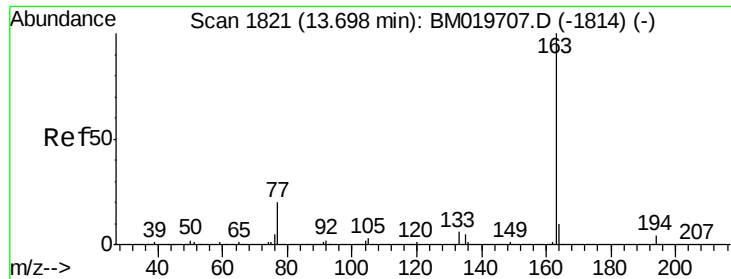

#45

Dimethylphthalate

Concen: 3.499 ng/ul

RT: 13.70 min Scan# 1821

Delta R.T. -0.01 min

Lab File: BM019713.D

Acq: 03 Apr 2019 04:26

Instrument :

BNA_M

ClientSampleId :

BF636



Tgt Ion:163 Resp: 122497

Ion Ratio Lower Upper

163 100

194 3.5 4.0 6.0#

164 10.7 8.4 12.6

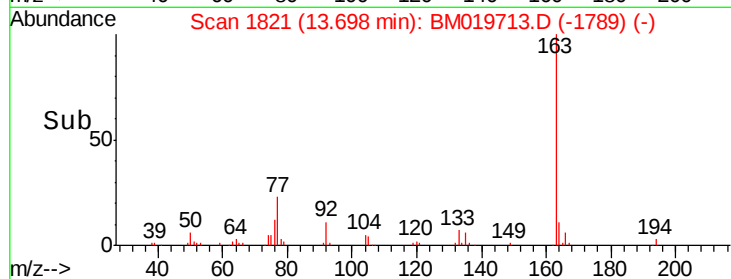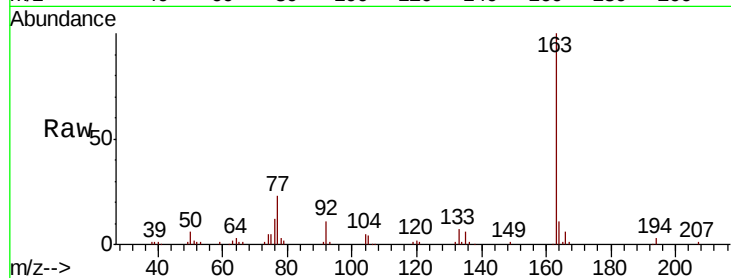

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

