

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040219\
 Data File : BM019724.D
 Acq On : 03 Apr 2019 11:26
 Operator : JU/SJ
 Sample : K2168-08
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF673

Quant Time: Apr 04 01:49:13 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 04 01:45:37 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	108704	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.35	136	506398	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.23	164	306825	20.00	ng/ul	-0.01
62) Phenanthrene-d10	16.99	188	705035	20.00	ng/ul	0.00
78) Chrysene-d12	21.20	240	724041	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	647995	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.12	96	18605	6.70	ng/uL	0.00
5) Phenol-d5	6.76	99	209509	21.64	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.92	67	139657	21.55	ng/ul	-0.01
9) 2-Chlorophenol-d4	7.10	132	169026	23.04	ng/ul	0.00
13) 4-Methylphenol-d8	8.29	113	178739	24.60	ng/ul	0.00
19) Nitrobenzene-d5	8.74	128	83048	22.99	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.46	143	96155	23.92	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	165694	21.84	ng/ul	0.00
29) 4-Chloroaniline-d4	10.52	131	212968	23.38	ng/ul	0.00
44) Dimethylphthalate-d6	13.65	166	614824	24.83	ng/ul	-0.01
47) Acenaphthylene-d8	13.92	160	717353	23.17	ng/ul	-0.01
52) 4-Nitrophenol-d4	14.49	143	72324	18.64	ng/ul	0.01
58) Fluorene-d10	15.23	176	508829	23.86	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	80370	17.24	ng/ul	0.00
71) Anthracene-d10	17.09	188	815425	24.10	ng/ul	-0.01
79) Pyrene-d10	19.40	212	861654	25.76	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	756636	22.03	ng/ul	0.00


Target Compounds					Qvalue	
45) Dimethylphthalate	13.70	163	126910	5.109	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040219\
Data File : BM019724.D
Acq On : 03 Apr 2019 11:26
Operator : JU/SJ
Sample : K2168-08
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF673

Quant Time: Apr 04 01:49:13 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 04 01:45:37 2019
Response via : Initial Calibration

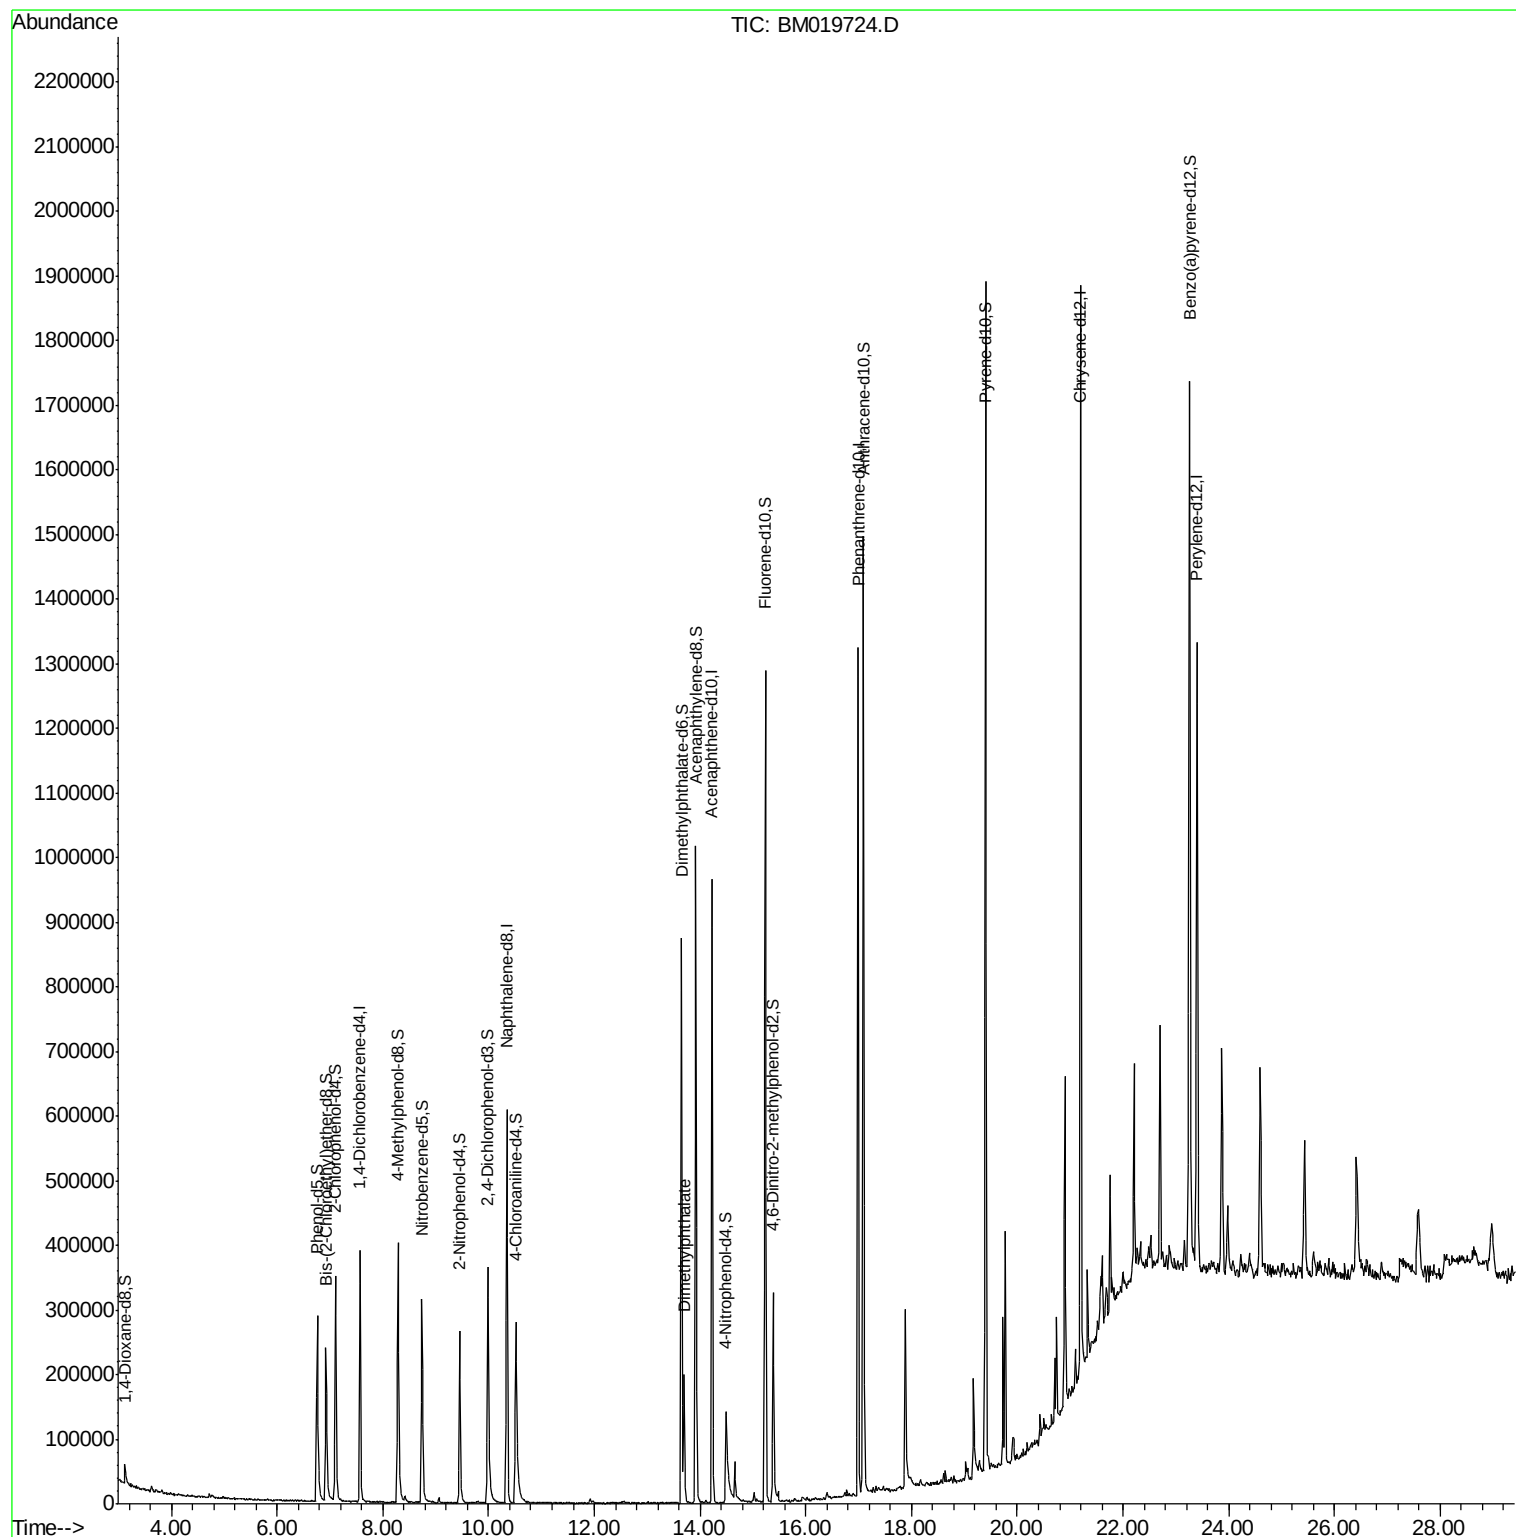

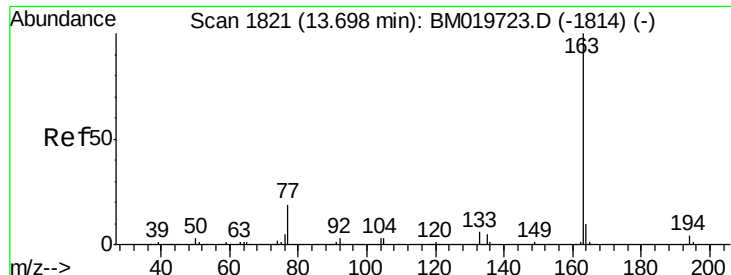

#45

Dimethylphthalate

Concen: 5.109 ng/ul

RT: 13.70 min Scan# 1821

Delta R.T. -0.01 min

Lab File: BM019724.D

Acq: 03 Apr 2019 11:26

Instrument :

BNA_M

ClientSampleId :

BF673


Tgt Ion:163 Resp: 126910

Ion Ratio Lower Upper

163 100

194 4.1 4.0 6.0

164 10.3 8.4 12.6

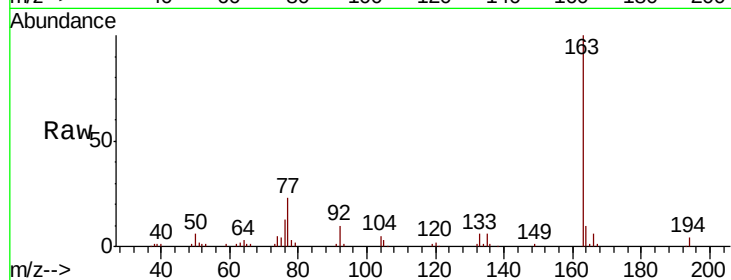

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

