

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040219\
 Data File : BM019727.D
 Acq On : 03 Apr 2019 13:16
 Operator : JU/SJ
 Sample : K2168-06
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF647

Manual Integrations
 APPROVED

Sohil
 4/4/2019 5:42:53 PM

Quant Time: Apr 04 02:02:45 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 04 01:45:37 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	154125	20.00	ng/ul	-0.02
18) Naphthalene-d8	10.35	136	719814	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.23	164	409144	20.00	ng/ul	-0.01
62) Phenanthrene-d10	16.99	188	877387	20.00	ng/ul	-0.01
78) Chrysene-d12	21.20	240	774268	20.00	ng/ul	0.00
86) Perylene-d12	23.40	264	679368	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.12	96	23945	6.08	ng/uL	0.00
5) Phenol-d5	6.75	99	266184	19.39	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	6.92	67	185145	20.15	ng/ul	-0.01
9) 2-Chlorophenol-d4	7.10	132	225123	21.64	ng/ul	-0.01
13) 4-Methylphenol-d8	8.28	113	185656	18.02	ng/ul	-0.01
19) Nitrobenzene-d5	8.74	128	106994	20.84	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.45	143	127545	22.32	ng/ul	-0.01
26) 2,4-Dichlorophenol-d3	9.98	165	220124	20.41	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.51	131	258173	19.94	ng/ul	-0.01
44) Dimethylphthalate-d6	13.65	166	759012	22.99	ng/ul	-0.02
47) Acenaphthylene-d8	13.92	160	893859	21.65	ng/ul	-0.01
52) 4-Nitrophenol-d4	14.49	143	75719m	14.63	ng/ul	0.01
58) Fluorene-d10	15.23	176	629735	22.14	ng/ul	-0.01
63) 4,6-Dinitro-2-methylphenol	15.38	200	81399	14.03	ng/ul	0.00
71) Anthracene-d10	17.09	188	901558	21.41	ng/ul	-0.01
79) Pyrene-d10	19.40	212	909405	25.43	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.26	264	685721	19.04	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.70	163	154110	4.653	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040219\
Data File : BM019727.D
Acq On : 03 Apr 2019 13:16
Operator : JU/SJ
Sample : K2168-06
Misc :
ALS Vial : 35 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BF647

Quant Time: Apr 04 02:02:45 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 04 01:45:37 2019
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
4/4/2019 5:42:53 PM

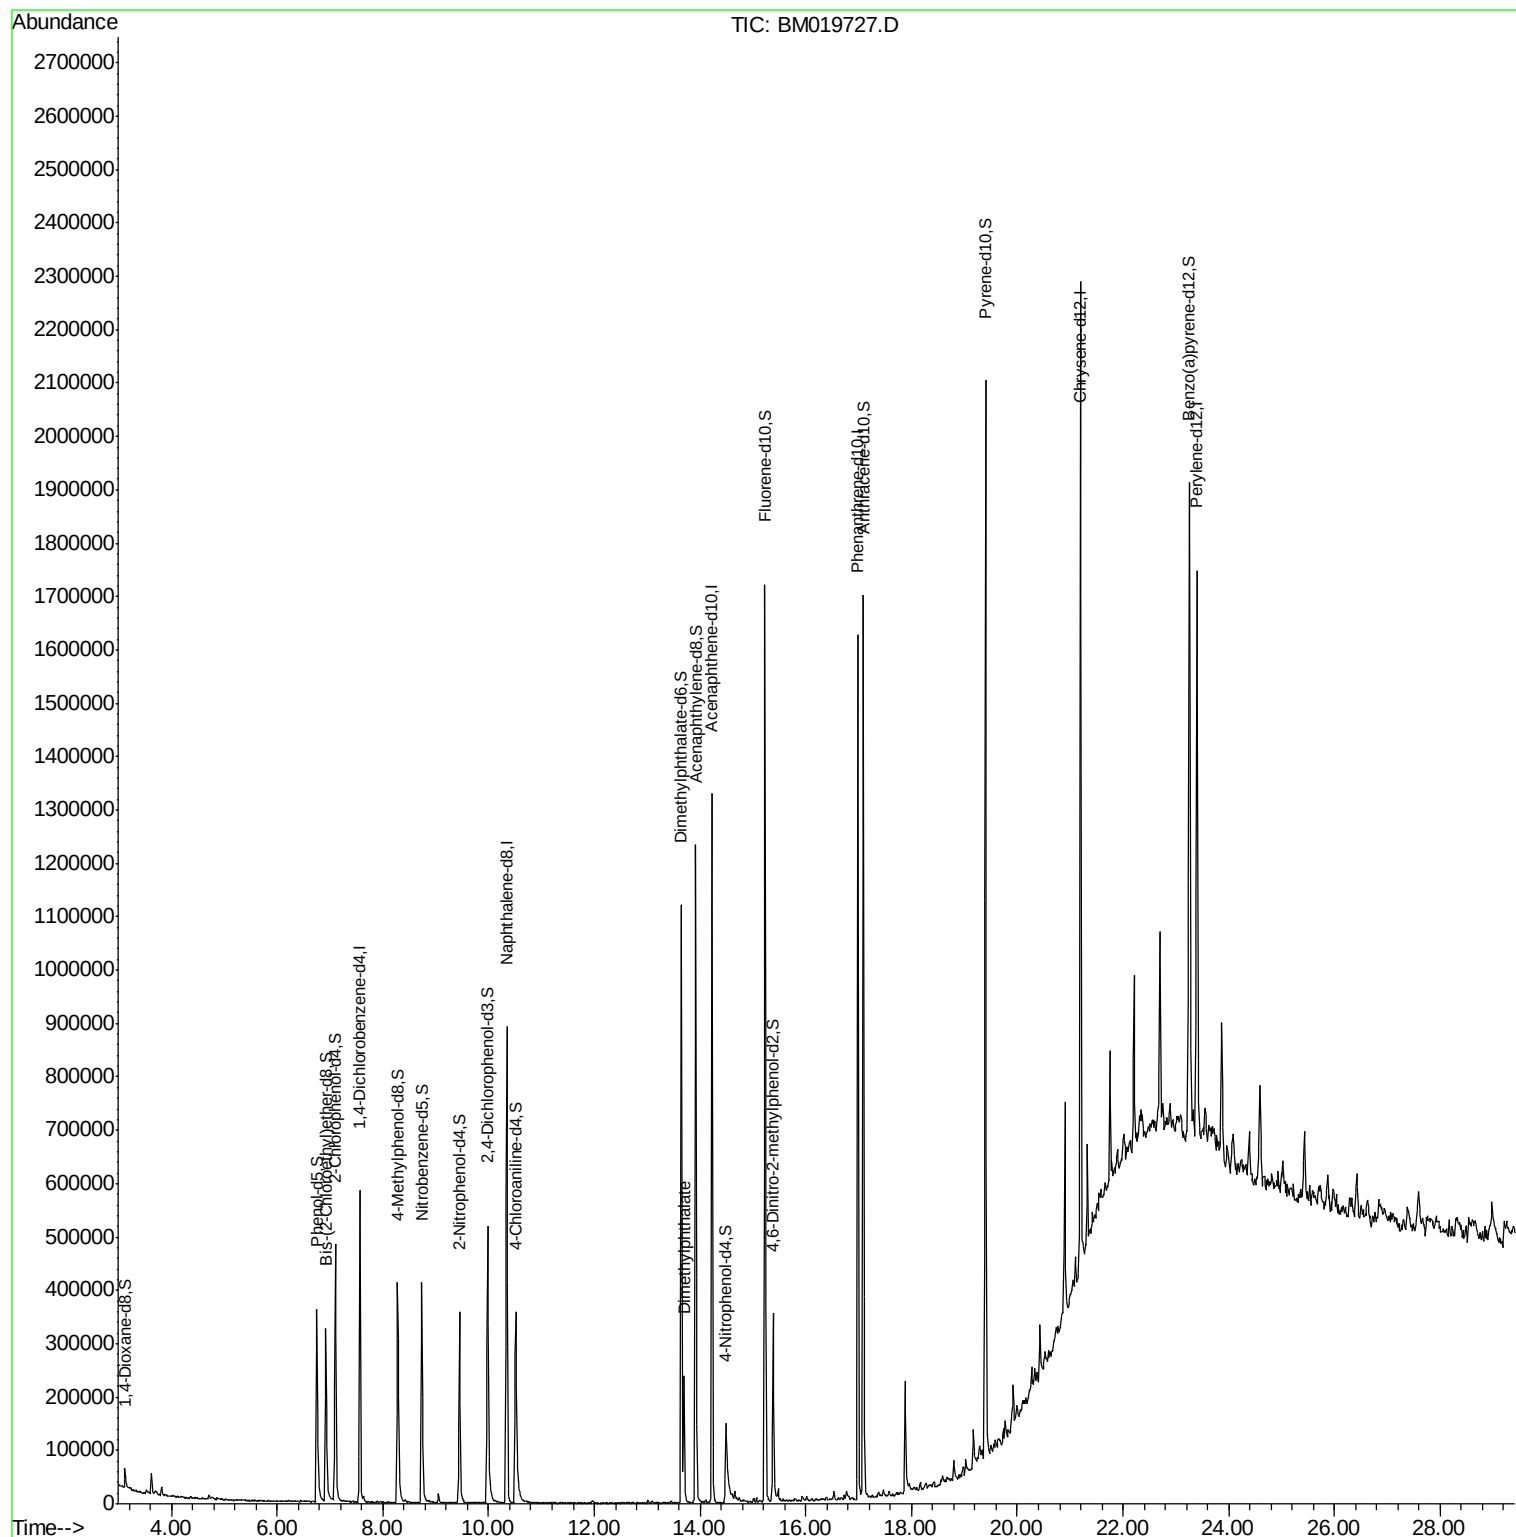

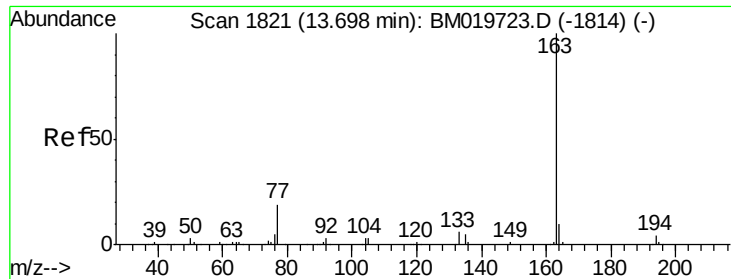

#45
 Dimethylphthalate
 Concen: 4.653 ng/ul
 RT: 13.70 min Scan# 1821
 Delta R.T. -0.01 min
 Lab File: BM019727.D
 Acq: 03 Apr 2019 13:16

Instrument :
 BNA_M
 ClientSampleId :
 BF647

Tgt Ion:	163	Resp:	154110
Ion Ratio		Lower	Upper
163	100		
194	4.1	4.0	6.0
164	10.7	8.4	12.6

Manual Integrations
 APPROVED

Sohil
 4/4/2019 5:42:53 PM

