

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040219\
 Data File : BM019737.D
 Acq On : 03 Apr 2019 19:23
 Operator : JU/SJ
 Sample : K2148-16DL 5X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF5J1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.452	77	79	82	rVB4	3868	3044	0.11%	0.015%
2	3.628	106	109	112	rBV3	7031	9466	0.33%	0.047%
3	4.252	213	215	219	rVB4	2984	3321	0.12%	0.016%
4	5.569	436	439	441	rBV3	3062	3916	0.14%	0.019%
5	6.769	637	643	656	rBV	39122	105121	3.69%	0.518%
6	6.928	664	670	687	rBV	39062	90784	3.18%	0.447%
7	7.104	694	700	712	rVB2	65398	121659	4.27%	0.599%
8	7.563	771	778	795	rBV	658306	1106796	38.82%	5.450%
9	8.298	897	903	920	rBV	47813	109848	3.85%	0.541%
10	8.751	974	980	992	rBV	52081	113252	3.97%	0.558%
11	9.063	1029	1033	1036	rVB2	3907	5190	0.18%	0.026%
12	9.457	1095	1100	1113	rBV	44939	95268	3.34%	0.469%
13	10.016	1187	1195	1208	rBV3	38662	121021	4.24%	0.596%
14	10.345	1244	1251	1265	rBV	1021075	1757423	61.64%	8.654%
15	10.551	1278	1286	1299	rBV2	22886	75908	2.66%	0.374%
16	13.651	1808	1813	1818	rBV	178219	274988	9.64%	1.354%
17	13.704	1818	1822	1834	rVB	41733	71340	2.50%	0.351%
18	13.922	1853	1859	1868	rBV	206933	326898	11.46%	1.610%
19	14.227	1904	1911	1922	rBV2	1555354	2361340	82.82%	11.628%
20	14.569	1963	1969	1974	rBV6	5920	17211	0.60%	0.085%
21	14.663	1982	1985	1995	rVB3	15845	26101	0.92%	0.129%
22	15.016	2040	2045	2049	rBV	5857	8235	0.29%	0.041%
23	15.069	2051	2054	2058	rBV4	4957	6618	0.23%	0.033%
24	15.233	2076	2082	2092	rBV	280018	443250	15.55%	2.183%
25	15.404	2106	2111	2117	rBV5	7190	12354	0.43%	0.061%
26	15.469	2120	2122	2126	rVB2	3173	4020	0.14%	0.020%
27	15.792	2172	2177	2178	rBV2	2537	3505	0.12%	0.017%
28	15.933	2195	2201	2202	rBV3	6387	7099	0.25%	0.035%
29	15.945	2202	2203	2211	rVB6	7424	10421	0.37%	0.051%
30	16.110	2227	2231	2233	rBV3	6122	6893	0.24%	0.034%
31	16.192	2242	2245	2248	rVB2	5710	6345	0.22%	0.031%
32	16.333	2266	2269	2273	rBV4	3361	5154	0.18%	0.025%
33	16.392	2275	2279	2286	rBV4	10312	19350	0.68%	0.095%
34	16.580	2308	2311	2312	rBV3	4024	4564	0.16%	0.022%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040219\
 Data File : BM019737.D
 Acq On : 03 Apr 2019 19:23
 Operator : JU/SJ
 Sample : K2148-16DL 5X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BF5J1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
 Title : SVOA CALIBRATION

35	16.645	2317	2322	2323	rBV4	2211	3041	0.11%	0.015%
36	16.751	2333	2340	2349	rBV3	53906	88180	3.09%	0.434%
37	16.863	2354	2359	2363	rVV2	18851	24343	0.85%	0.120%
38	16.892	2363	2364	2369	rVB4	2924	3132	0.11%	0.015%
39	16.992	2374	2381	2392	rBV2	1902019	2748042	96.38%	13.532%
40	17.092	2392	2398	2408	rVB2	298340	481620	16.89%	2.372%
41	17.198	2414	2416	2421	rVB4	3701	4246	0.15%	0.021%
42	17.280	2425	2430	2433	rBV3	3122	5357	0.19%	0.026%
43	17.421	2452	2454	2458	rBV4	4006	5833	0.20%	0.029%
44	17.468	2458	2462	2466	rVV6	4981	7324	0.26%	0.036%
45	17.615	2482	2487	2490	rBV6	4319	6688	0.23%	0.033%
46	17.710	2499	2503	2509	rBV3	14685	25662	0.90%	0.126%
47	17.768	2509	2513	2514	rVV4	4184	5259	0.18%	0.026%
48	17.821	2518	2522	2527	rVV2	31592	43095	1.51%	0.212%
49	17.880	2527	2532	2540	rVV2	106624	177365	6.22%	0.873%
50	17.957	2541	2545	2551	rVB	103646	131395	4.61%	0.647%
51	18.057	2560	2562	2569	rVB7	6655	11585	0.41%	0.057%
52	18.163	2577	2580	2583	rBV4	12945	15562	0.55%	0.077%
53	18.439	2625	2627	2633	rVB6	8204	9142	0.32%	0.045%
54	18.751	2677	2680	2683	rBV4	11441	15150	0.53%	0.075%
55	18.804	2687	2689	2693	rVB5	9307	9511	0.33%	0.047%
56	19.062	2728	2733	2738	rBV	71207	111781	3.92%	0.550%
57	19.174	2748	2752	2755	rBV	46190	72896	2.56%	0.359%
58	19.398	2785	2790	2794	rBV2	383787	574596	20.15%	2.829%
59	19.698	2839	2841	2845	rVB	24193	25436	0.89%	0.125%
60	20.192	2923	2925	2928	rVB	58047	55474	1.95%	0.273%
61	20.333	2945	2949	2954	rBV	2597039	2851282	100.00%	14.041%
62	21.103	3076	3080	3085	rBV	602636	645846	22.65%	3.180%
63	21.198	3091	3096	3101	rBV	2082140	2631187	92.28%	12.957%
64	23.403	3466	3471	3486	rVB	1131366	2179650	76.44%	10.733%


Sum of corrected areas: 20307383

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040219\
Data File : BM019737.D
Acq On : 03 Apr 2019 19:23
Operator : JU/SJ
Sample : K2148-16DL 5X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF5J1DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

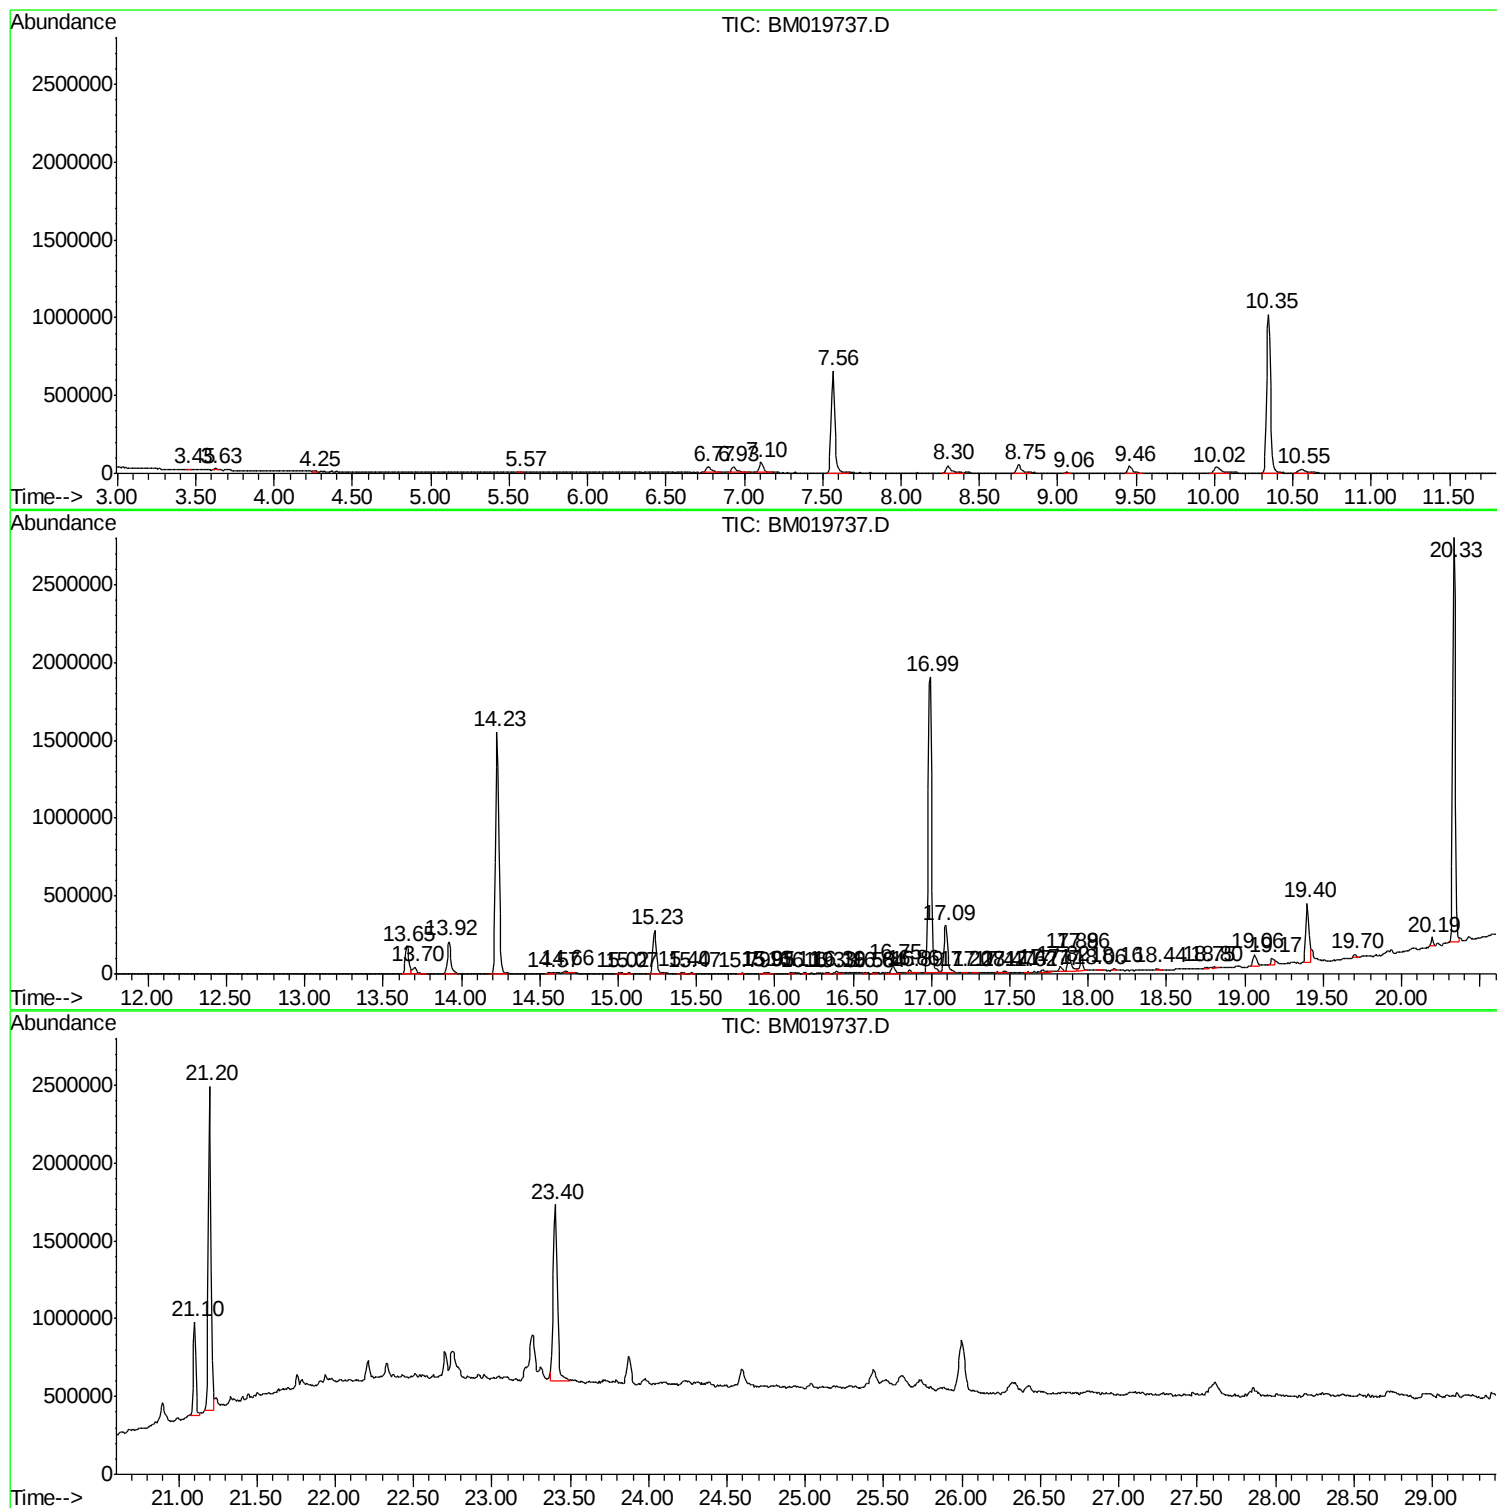

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040219\
Data File : BM019737.D
Acq On : 03 Apr 2019 19:23
Operator : JU/SJ
Sample : K2148-16DL 5X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF5J1DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM040219\
Data File : BM019737.D
Acq On : 03 Apr 2019 19:23
Operator : JU/SJ
Sample : K2148-16DL 5X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BF5J1DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM032219MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc