
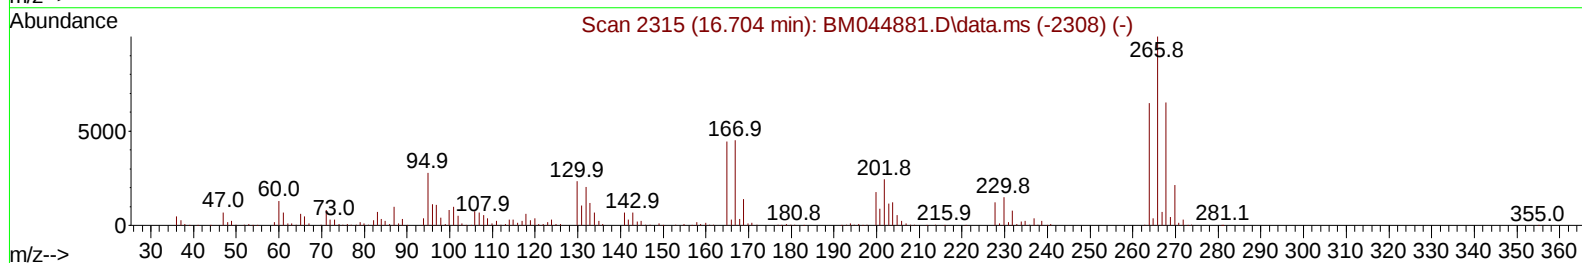
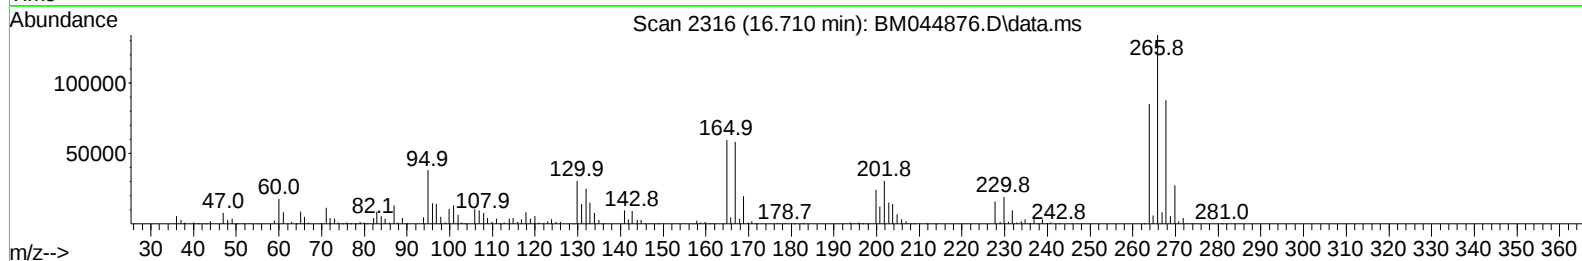


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040224\
Data File : BM044876.D
Acq On : 02 Apr 2024 12:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 03 00:41:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 03 00:28:57 2024
Response via : Initial Calibration

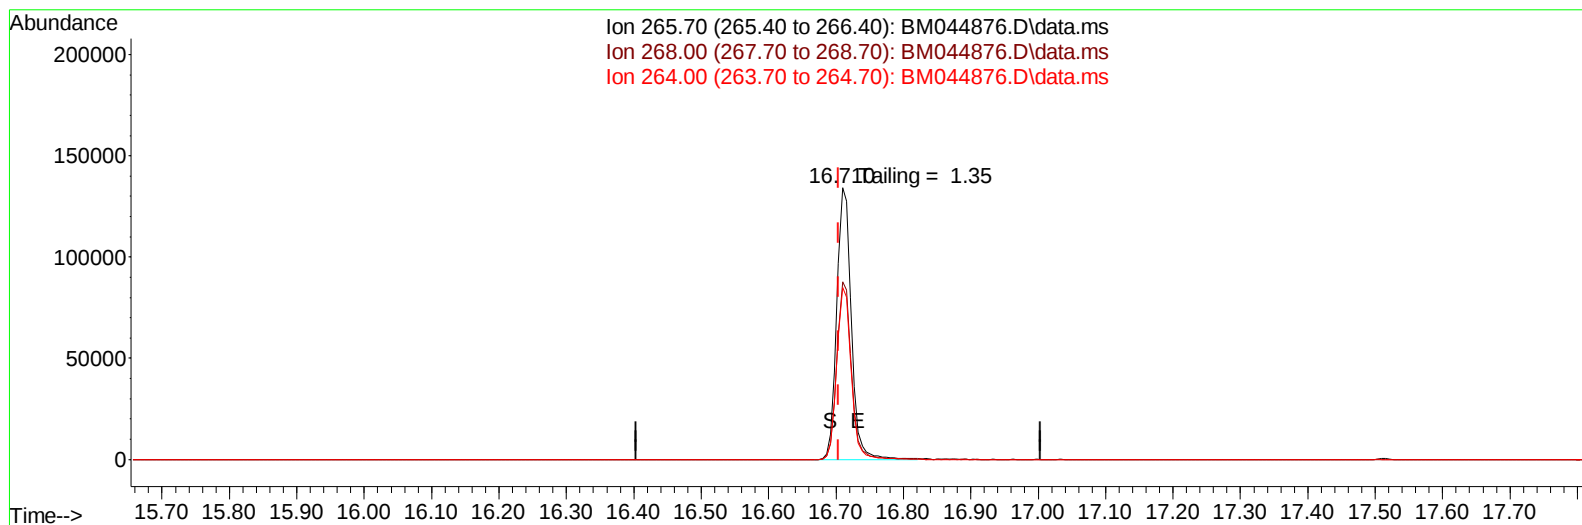

TIC: BM044876.D\data.ms




(70) Pentachlorophenol (C)

16.710min (+ 0.006) 0.00 ng

response 201059

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.00	65.51
264.00	64.60	63.36
0.00	0.00	0.00

Quant Time: Apr 03 00:41:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : wed Apr 03 00:28:57 2024
Response via : Initial Calibration

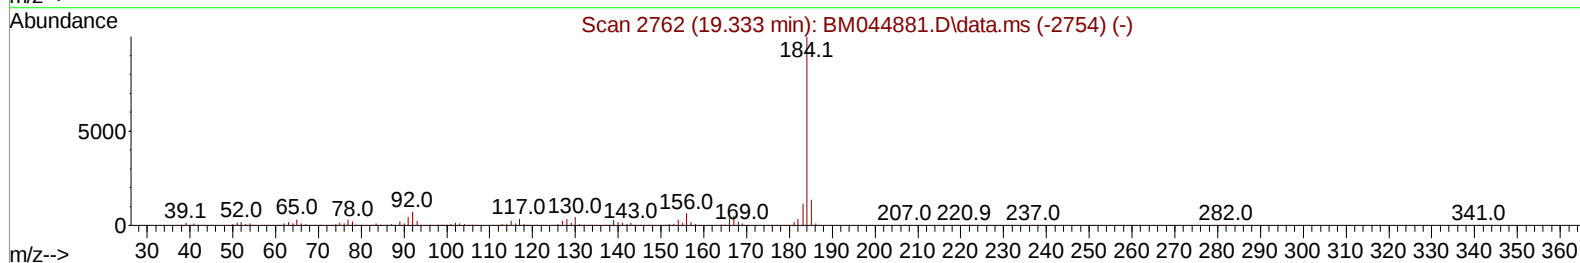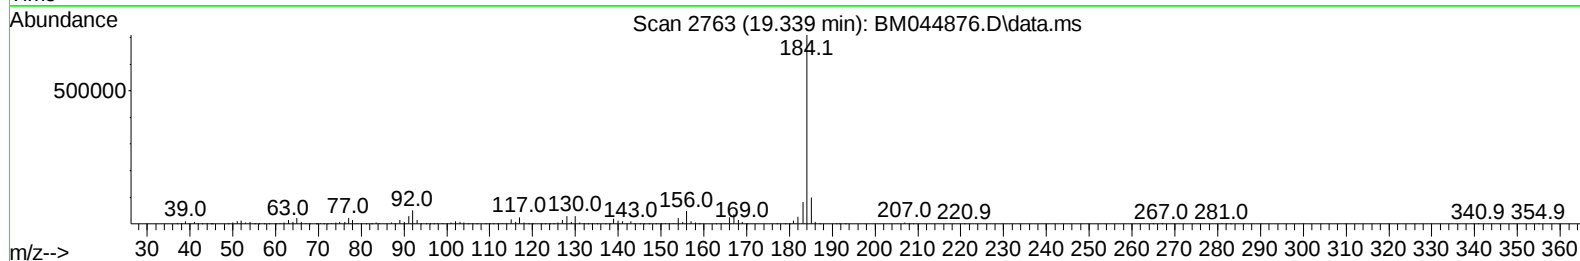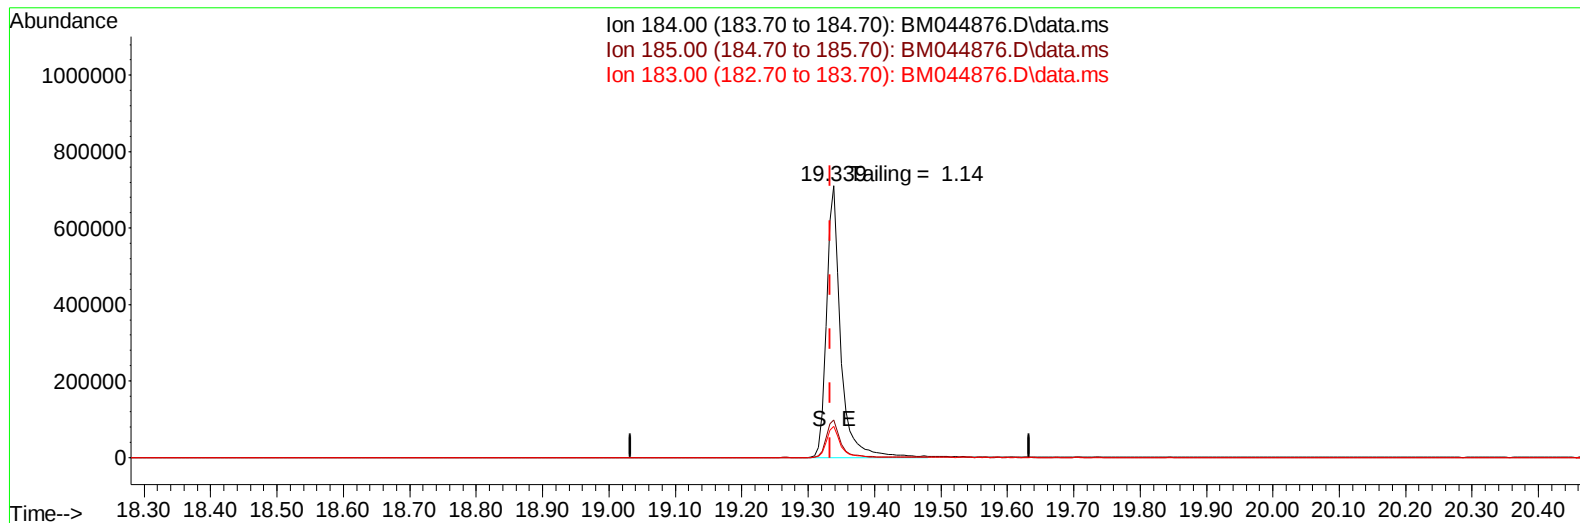

TIC: BM044876.D\data.ms

(77) Benzidine

19.339min (+ 0.006) 31074.81 ng

response **1055495**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.84
183.00	11.60	11.49
0.00	0.00	0.00