


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040224\
Data File : BM044876.D
Acq On : 02 Apr 2024 12:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040224.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Apr 03 00:28:57 2024

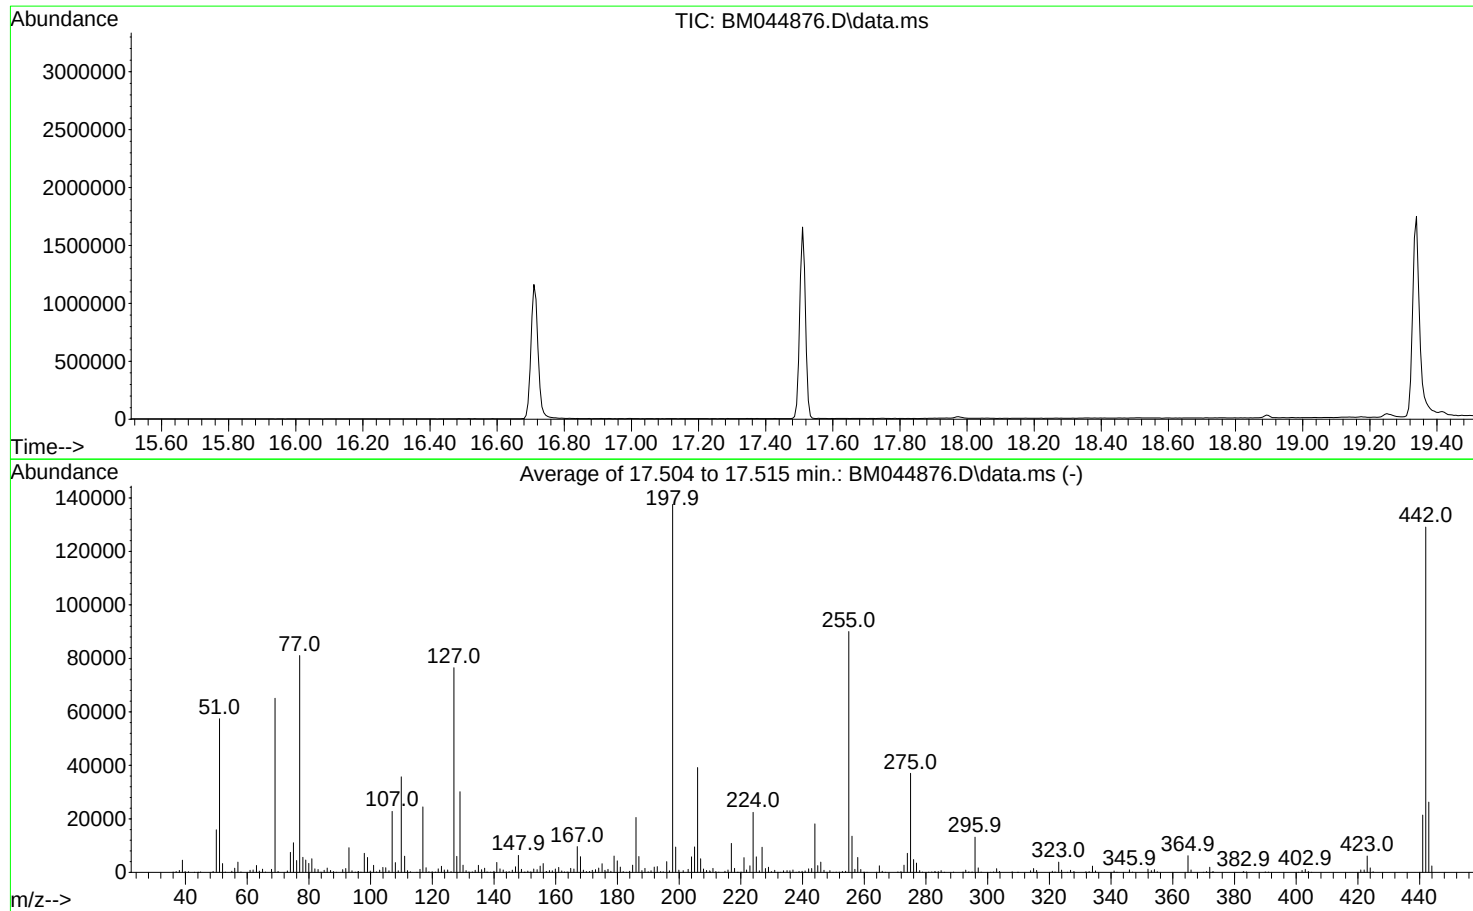




AutoFind: Scans 2451, 2452, 2453; Background Corrected with Scan 2444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.8	57452	PASS
68	69	0.00	2	1.7	1134	PASS
69	198	0.00	100	47.3	65085	PASS
70	69	0.00	2	0.6	362	PASS
127	198	10	80	55.6	76501	PASS
197	198	0.00	2	0.5	628	PASS
198	198	100	100	100.0	137525	PASS
199	198	5	9	6.9	9462	PASS
275	198	10	60	26.9	37016	PASS
365	198	1	100	4.5	6245	PASS
441	198	0.01	100	15.6	21399	PASS
442	442	50	100	100.0	129093	PASS
443	442	15	24	20.3	26259	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040224\
Data File : BM044876.D
Acq On : 02 Apr 2024 12:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 03 00:41:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 03 00:28:57 2024
Response via : Initial Calibration

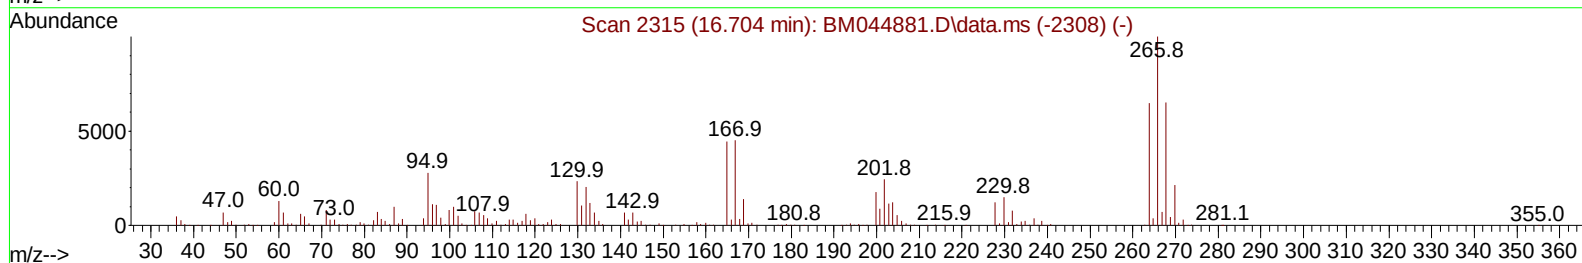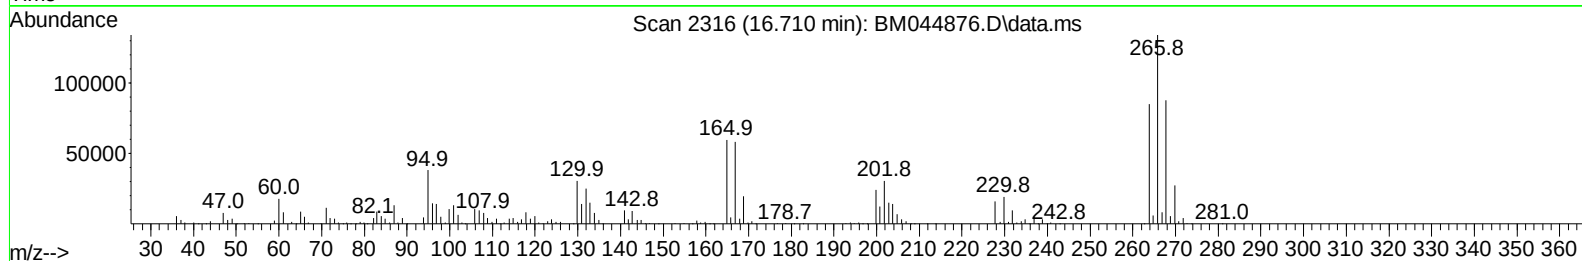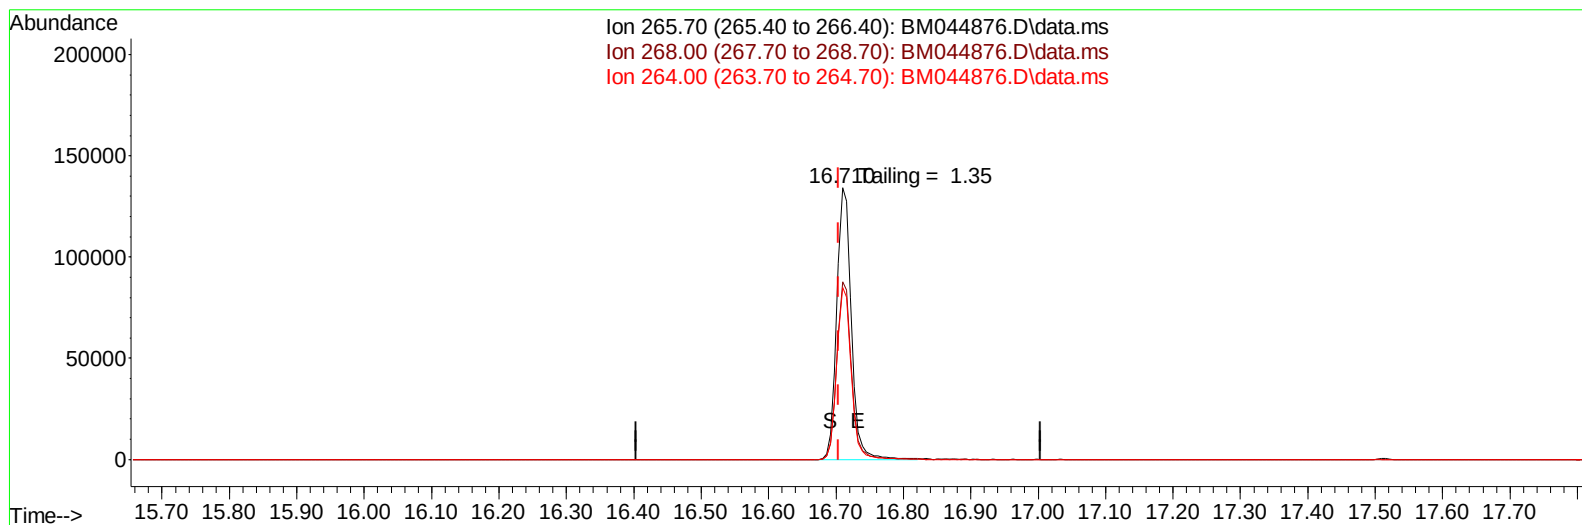

TIC: BM044876.D\data.ms

(70) Pentachlorophenol (C)

16.710min (+ 0.006) 0.00 ng




response 201059

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.00	65.51
264.00	64.60	63.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040224\
Data File : BM044876.D
Acq On : 02 Apr 2024 12:57
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 03 00:41:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 03 00:28:57 2024
Response via : Initial Calibration

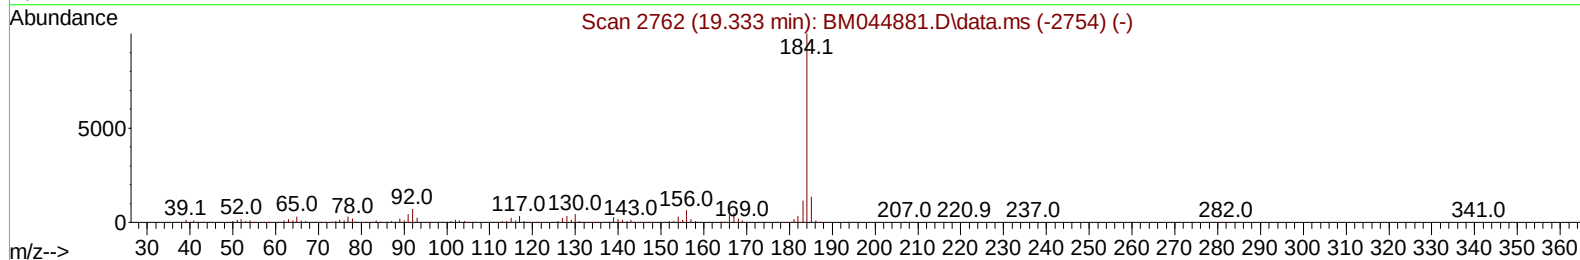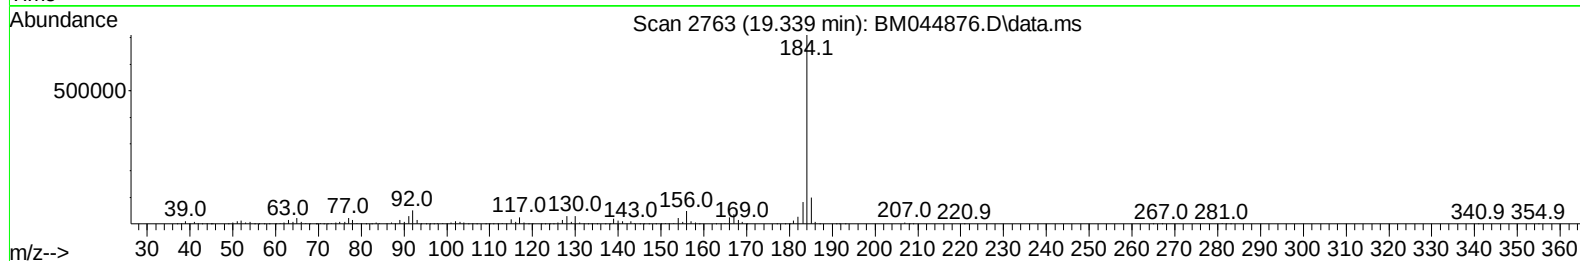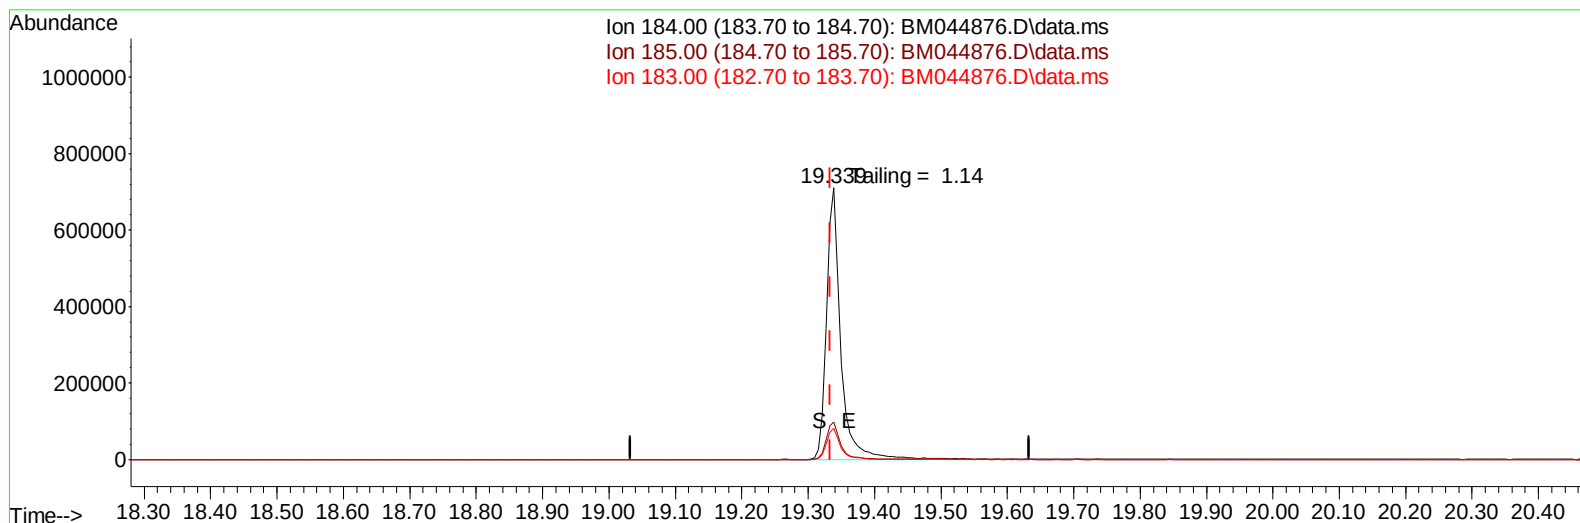

TIC: BM044876.D\data.ms

(77) Benzidine

19.339min (+ 0.006) 31074.81 ng

response 1055495

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.84
183.00	11.60	11.49
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/2/2024	BNA_M	<u>BM044876.D</u>
Compound Name	Response	Retention Time
DDT	684787	20.568
DDD	5736	20.174
DDE	0	19.856
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5736	690523	0.83

Instrument :
BNA_M
ClientSampleId :
DFTPP