

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040324\
Data File : BM044889.D
Acq On : 03 Apr 2024 10:30
Operator : MA/JU
Sample : PB159882BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB159882BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040224.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM044889.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.257	363	369	383	rBV	2128509	2982758	43.57%	10.923%
2	6.828	629	636	650	rBV	1894015	2935191	42.88%	10.749%
3	7.645	769	775	785	rVB	333825	526408	7.69%	1.928%
4	8.810	965	973	982	rBV	995286	1682700	24.58%	6.162%
5	10.422	1236	1247	1260	rBV	351358	662094	9.67%	2.425%
6	12.910	1663	1670	1687	rBV	2593107	3835884	56.04%	14.048%
7	14.298	1899	1906	1916	rBV	522856	844783	12.34%	3.094%
8	15.798	2154	2161	2175	rBV	2136062	3209483	46.89%	11.754%
9	17.057	2368	2375	2388	rBV	648263	1017286	14.86%	3.725%
10	19.704	2819	2825	2836	rBV	5833224	6845305	100.00%	25.068%
11	21.262	3085	3090	3099	rBV	923787	1271235	18.57%	4.655%
12	23.492	3463	3469	3481	rVB	763201	1493390	21.82%	5.469%




Sum of corrected areas: 27306517

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040324\
Data File : BM044889.D
Acq On : 03 Apr 2024 10:30
Operator : MA/JU
Sample : PB159882BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB159882BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

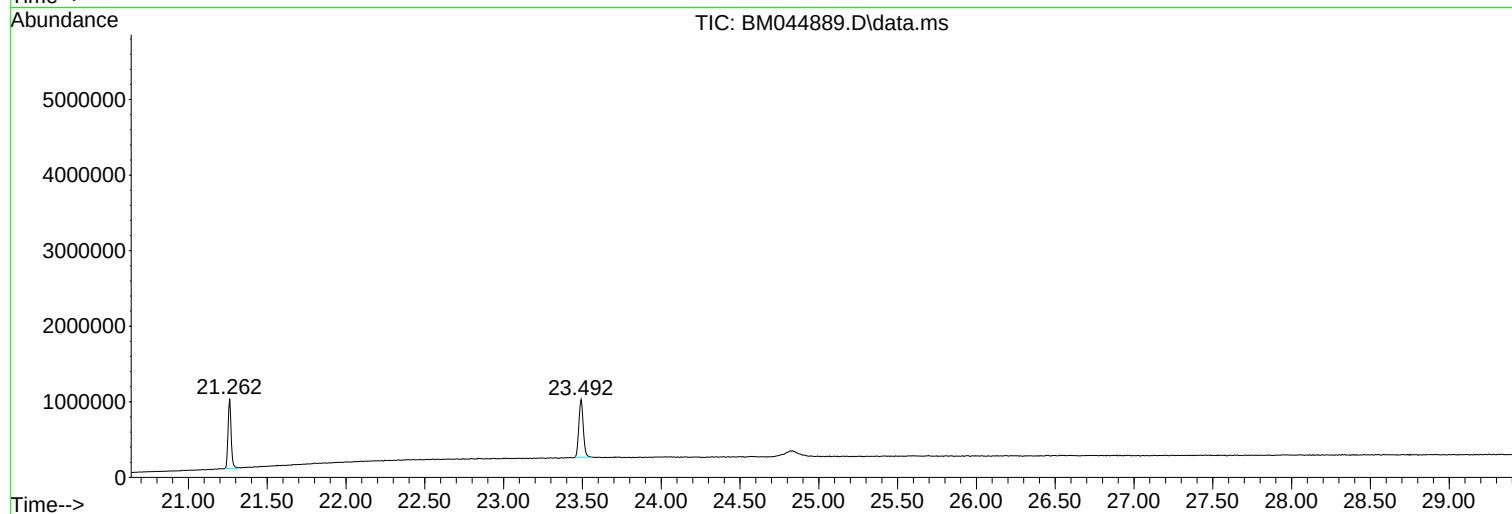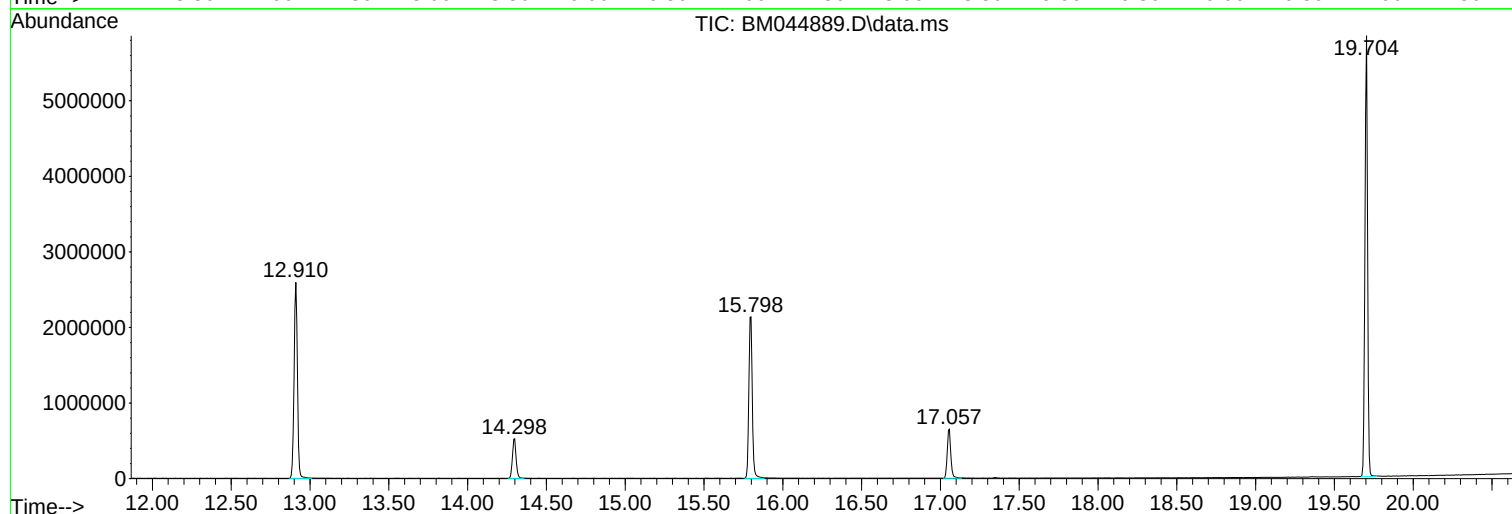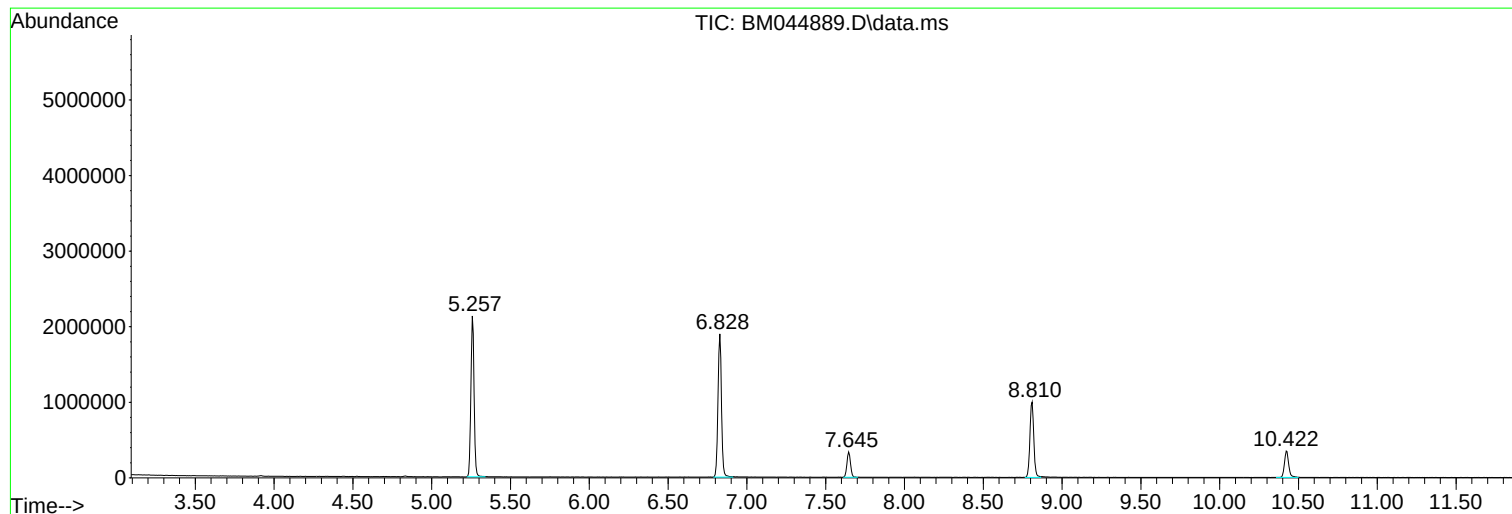

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040324\
Data File : BM044889.D
Acq On : 03 Apr 2024 10:30
Operator : MA/JU
Sample : PB159882BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB159882BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040324\
Data File : BM044889.D
Acq On : 03 Apr 2024 10:30
Operator : MA/JU
Sample : PB159882BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB159882BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------