
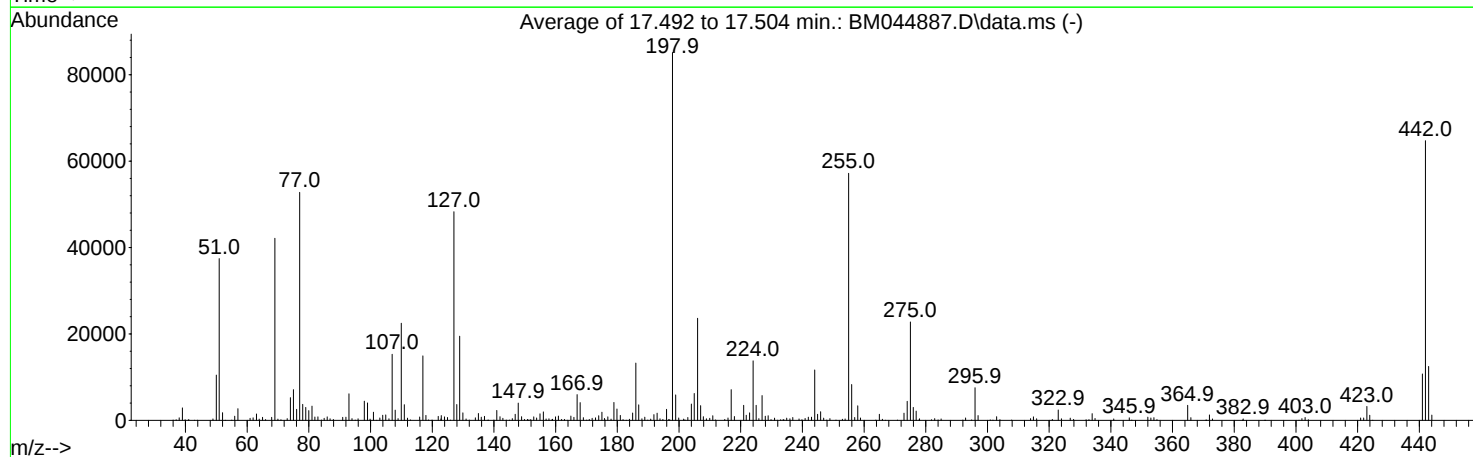


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040324\
Data File : BM044887.D
Acq On : 03 Apr 2024 09:18
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040224.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Apr 03 00:28:57 2024

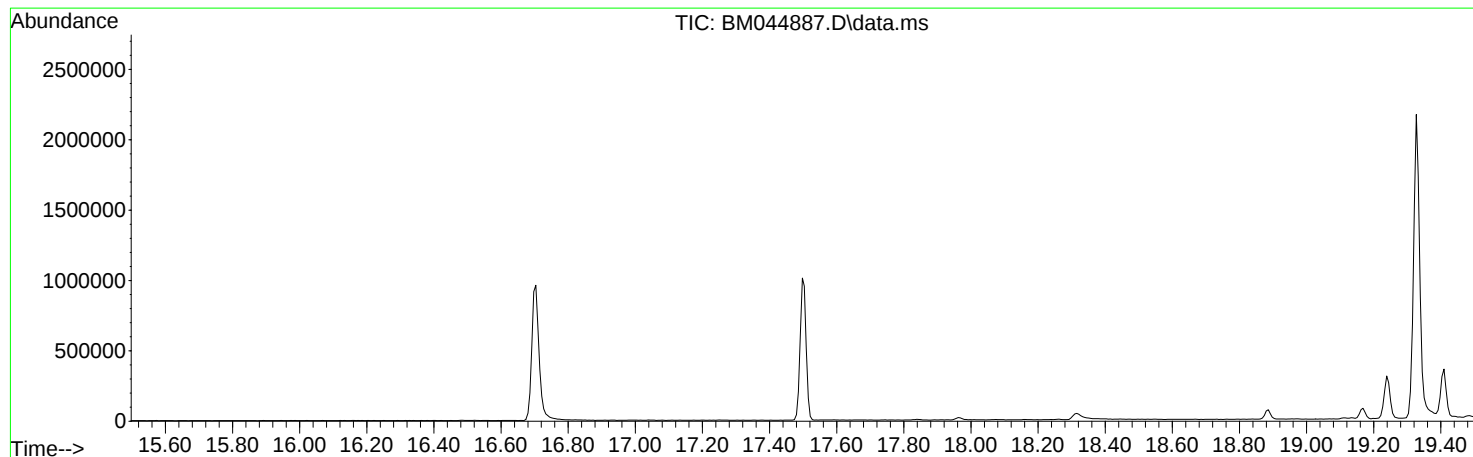




AutoFind: Scans 2449, 2450, 2451; Background Corrected with Scan 2443

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.0	37439	PASS
68	69	0.00	2	1.7	713	PASS
69	198	0.00	100	49.5	42136	PASS
70	69	0.00	2	0.7	294	PASS
127	198	10	80	56.7	48280	PASS
197	198	0.00	2	0.3	236	PASS
198	198	100	100	100.0	85147	PASS
199	198	5	9	6.9	5891	PASS
275	198	10	60	26.7	22761	PASS
365	198	1	100	4.1	3481	PASS
441	198	0.01	100	12.6	10732	PASS
442	442	50	100	100.0	64749	PASS
443	442	15	24	19.3	12499	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040324\
Data File : BM044887.D
Acq On : 03 Apr 2024 09:18
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 04 00:09:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 03 00:28:57 2024
Response via : Initial Calibration

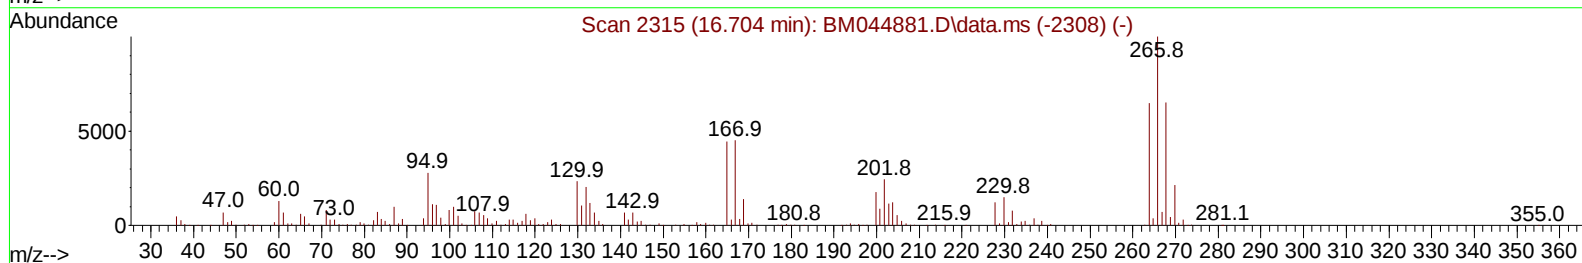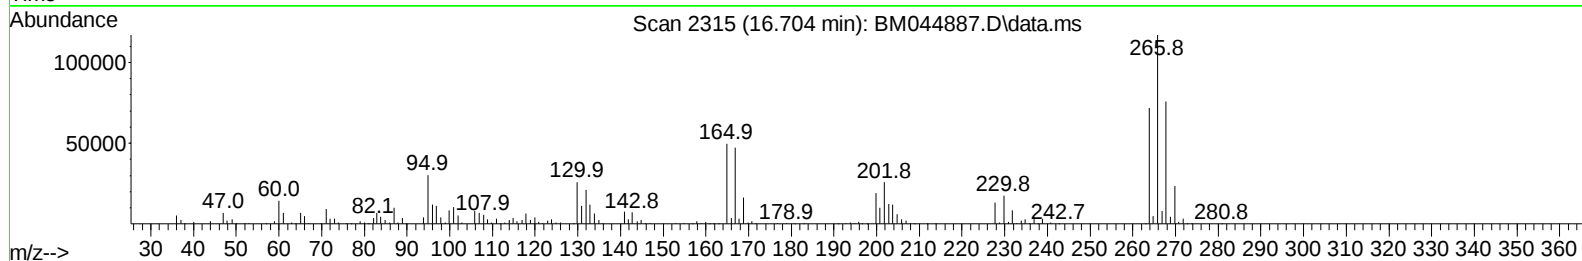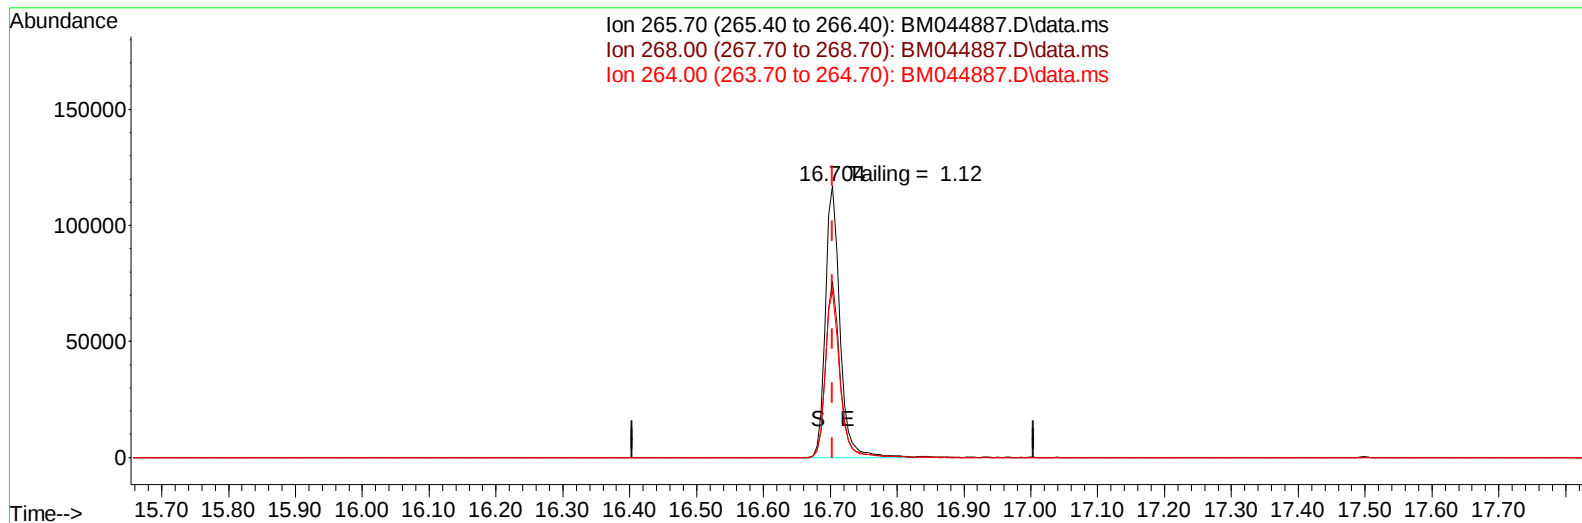

TIC: BM044887.D\data.ms

(70) Pentachlorophenol (C)

16.704min (-0.000) 0.00 ng




response 175538

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.00	64.66
264.00	64.60	61.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040324\
Data File : BM044887.D
Acq On : 03 Apr 2024 09:18
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 04 00:09:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040224.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 03 00:28:57 2024
Response via : Initial Calibration

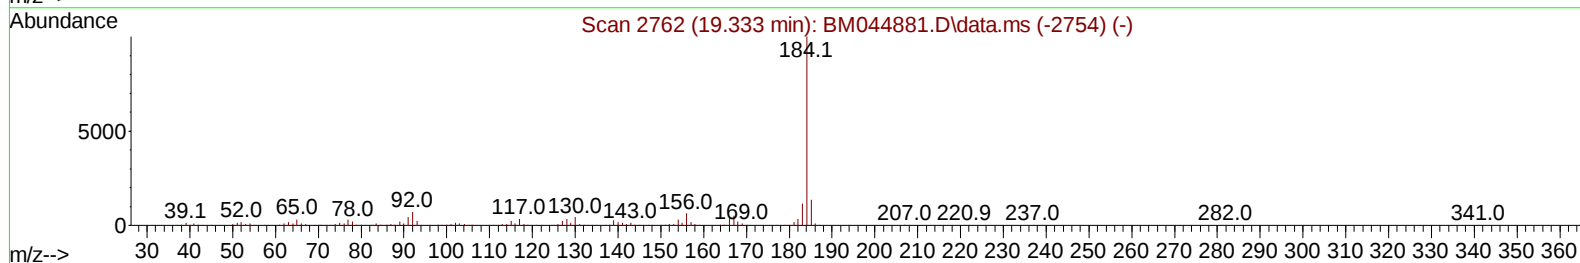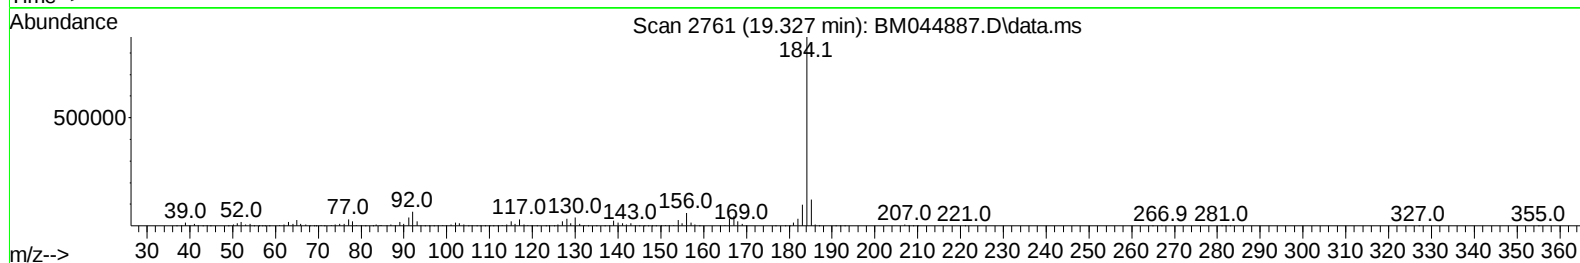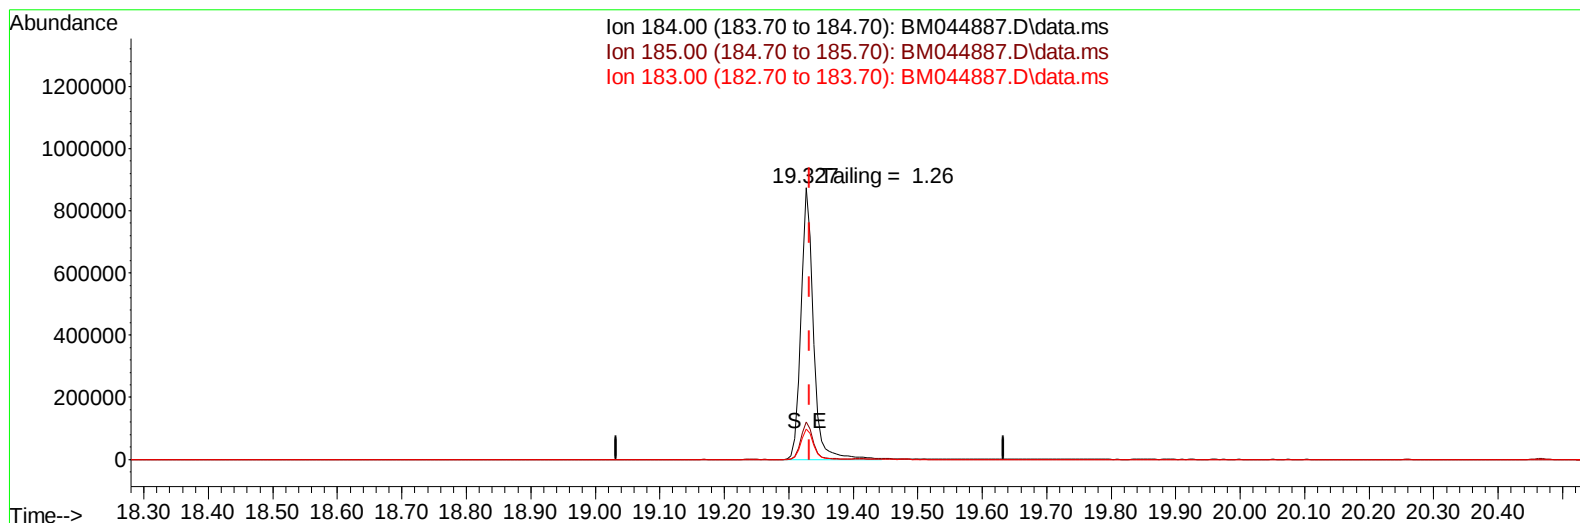

TIC: BM044887.D\data.ms

(77) Benzidine

19.327min (-0.006) 236007.39 ng

response 1162802

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.81
183.00	11.60	11.32
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/3/2024	BNA_M	<u>BM04487.D</u>
Compound Name	Response	Retention Time
DDT	583262	20.562
DDD	6303	20.168
DDE	0	19.856
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6303	589565	1.07

Instrument :
BNA_M
ClientSampleId :
DFTPP