

Quantitation Report (QT Reviewed)


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM040420\
 Data File : BM025908.D
 Acq On : 03 Apr 2020 12:03
 Operator : CG/JU
 Sample : PB127932BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 SBLK32

Manual Integrations
 APPROVED

mohammad
 4/6/2020 1:40:17 PM

Quant Time: Apr 03 12:36:22 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM040220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 02 10:49:07 2020
 Response via : Initial Calibration

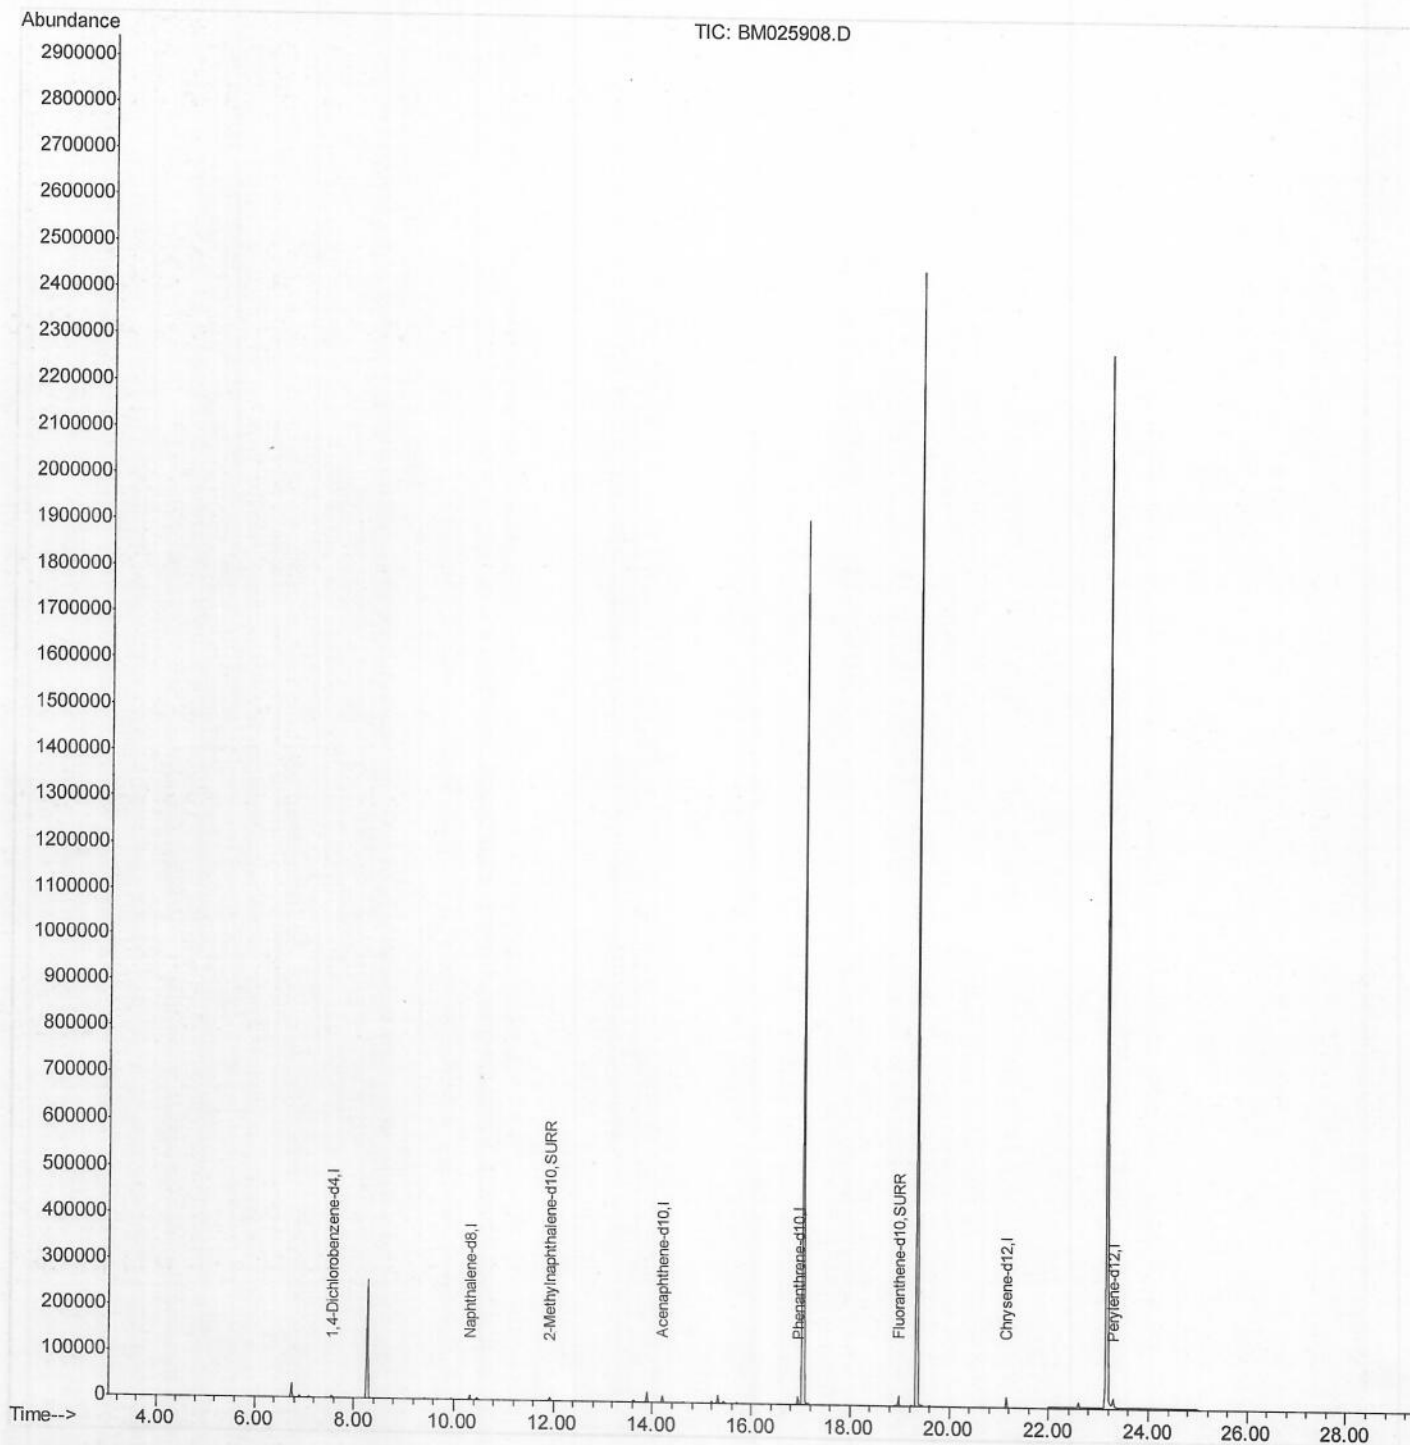

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM040420\
 Data File : BM025908.D
 Acq On : 03 Apr 2020 12:03
 Operator : CG/JU
 Sample : PB127932BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK32

Manual Integrations
 APPROVED

mohammad
 4/6/2020 1:40:17 PM

Quant Time: Apr 03 12:35:10 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM040220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 02 10:49:07 2020
 Response via : Initial Calibration

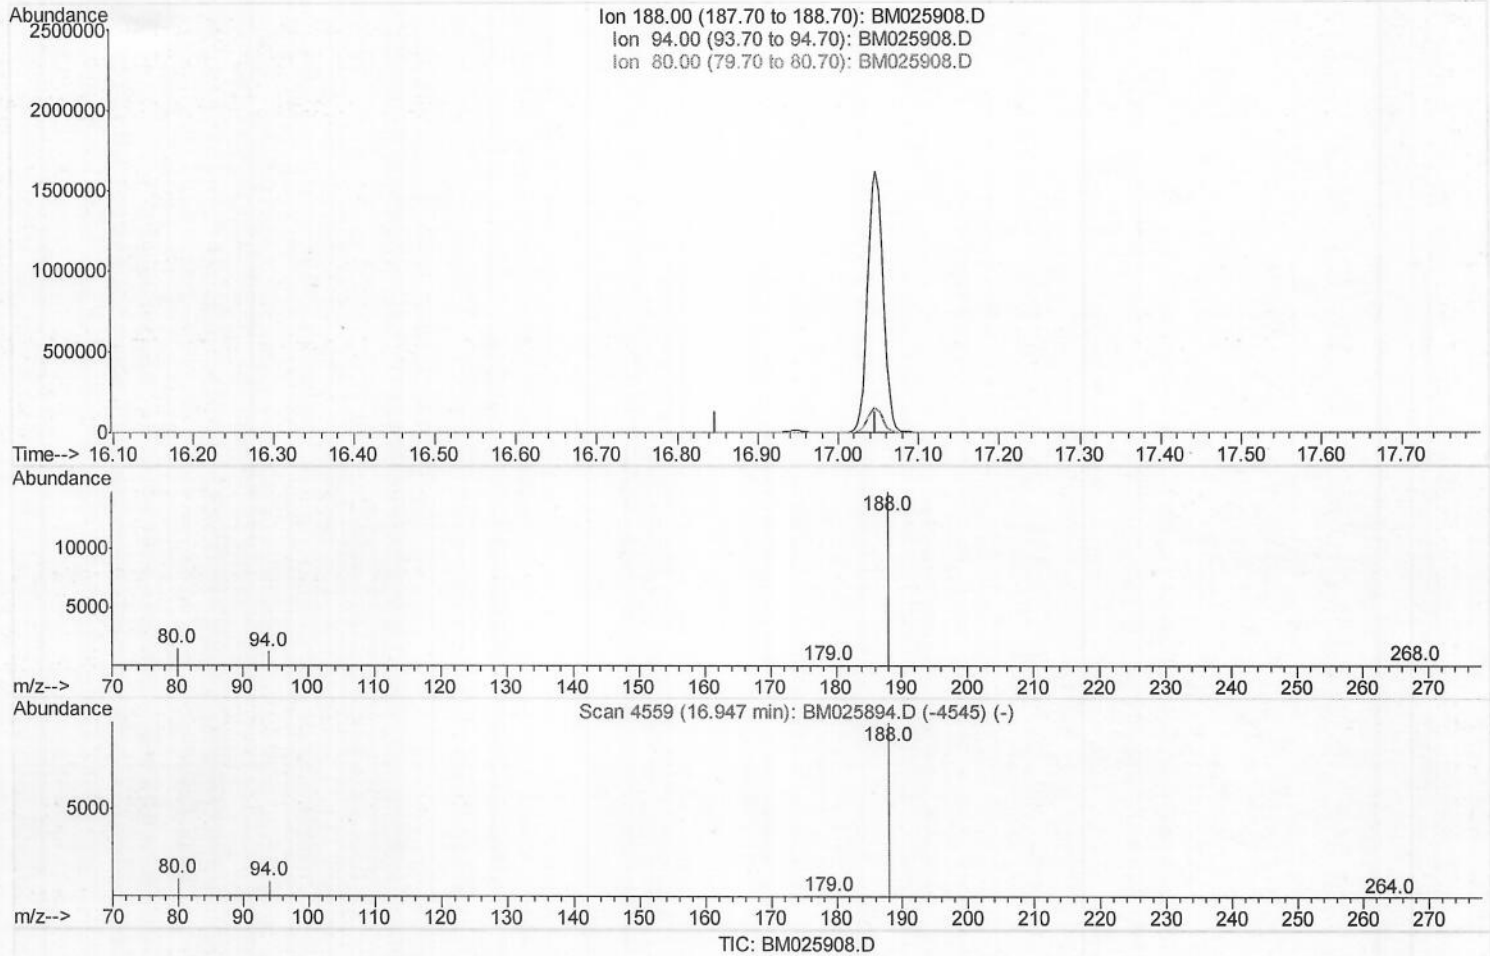

(10) Phenanthrene-d10 (I)

16.947min (-16.947) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	8.20	0.00#
80.00	9.50	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM040420\
 Data File : BM025908.D
 Acq On : 03 Apr 2020 12:03
 Operator : CG/JU
 Sample : PB127932BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 SBLK32

Manual Integrations
 APPROVED

mohammad
 4/6/2020 1:40:17 PM

Quant Time: Apr 03 12:35:10 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM040220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 02 10:49:07 2020
 Response via : Initial Calibration

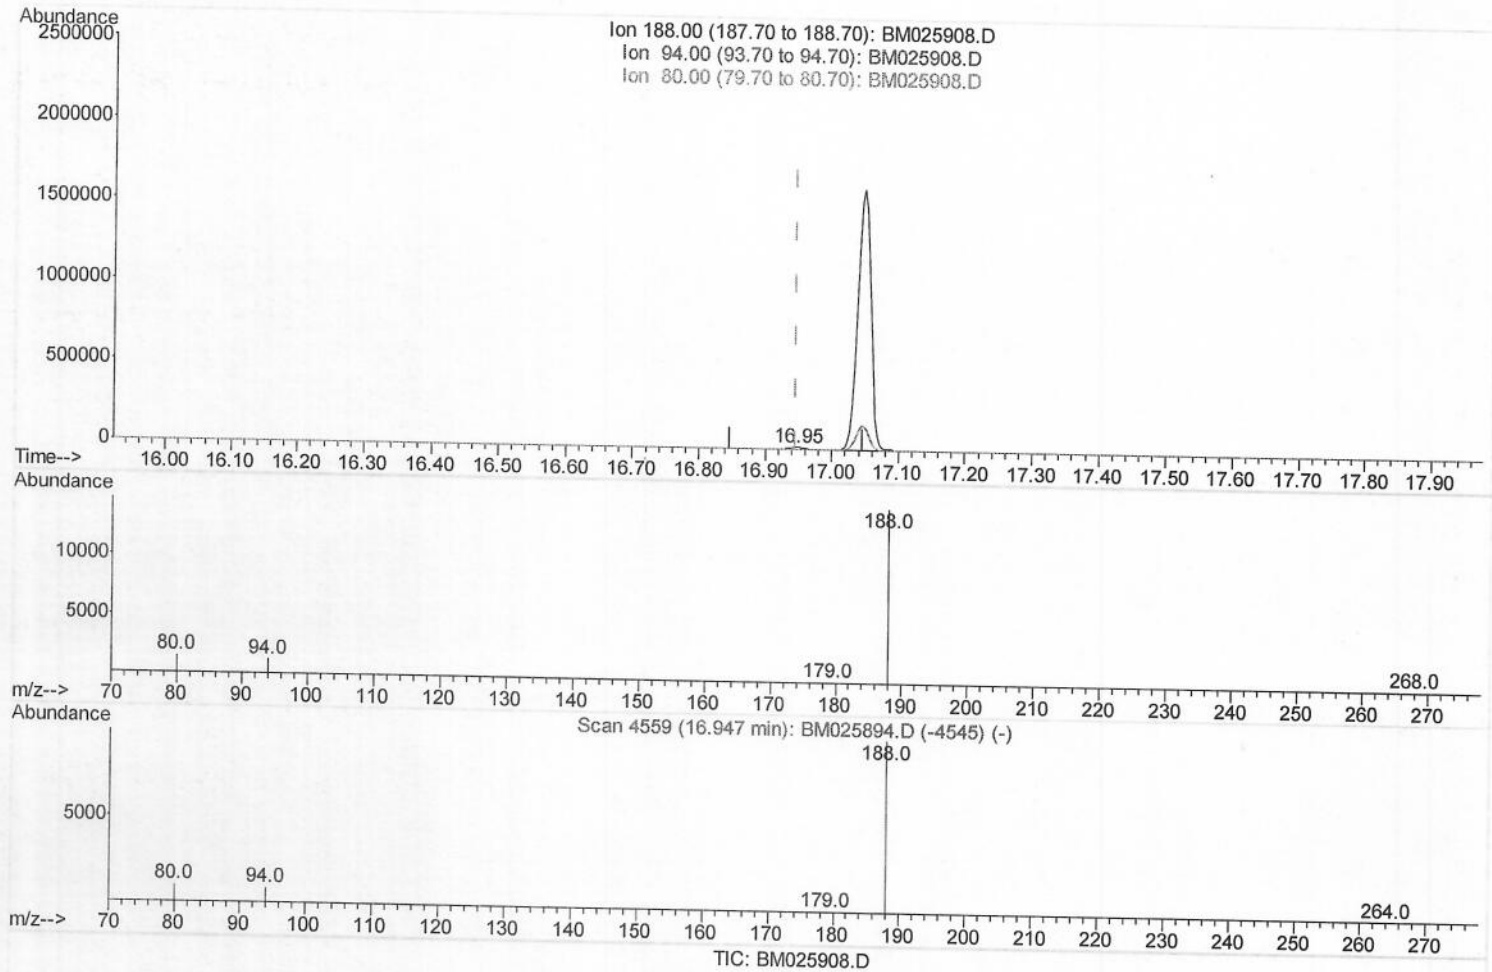

(10) Phenanthrene-d10 (I)

16.947min (+0.000) 0.40ng/ul m

response 19787

Ion	Exp%	Act%
188.00	100	100
94.00	8.20	8.46
80.00	9.50	10.05
0.00	0.00	0.00

AP
 04/20/2020

Quantitation Report (QT Reviewed)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM040420\
 Data File : BM025908.D
 Acq On : 03 Apr 2020 12:03
 Operator : CG/JU
 Sample : PB127932BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 Client Sampled :
 SBLK32

Manual Integrations
 APPROVED

mohammad
 4/6/2020 1:40:17 PM

Quant Time: Apr 03 12:36:22 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM040220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 02 10:49:07 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.57	152	2649	0.40	ng/ul	0.00
2) Naphthalene-d8	10.33	136	11607	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.20	164	8554	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.95	188	19787m	0.40	ng/ul	0.00
16) Chrysene-d12	21.14	240	20712	0.40	ng/ul	0.00
20) Perylene-d12	23.29	264	23154	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.93	152	8831	0.43	ng/ul	0.00
14) Fluoranthene-d10	18.98	212	26146	0.42	ng/ul	0.00

AP
 04/10/2020

Target Compounds

(#) = qualifier out of range (m) = manual integration (+) = signals summed