

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM040420\
 Data File : BM025925.D
 Acq On : 03 Apr 2020 22:59
 Operator : CG/JU
 Sample : PB127888BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK88

Manual Integrations
 APPROVED

mohammad
 4/6/2020 1:41:15 PM

Quant Time: Apr 04 00:30:09 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM040220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 03 22:53:21 2020
 Response via : Initial Calibration

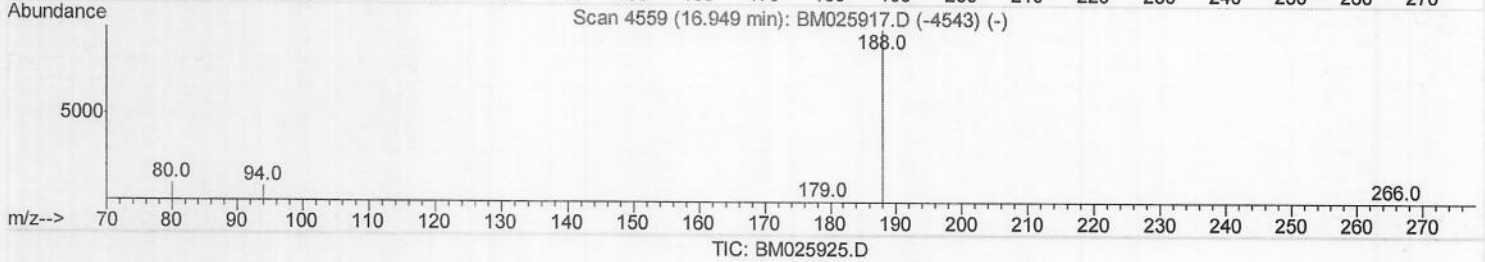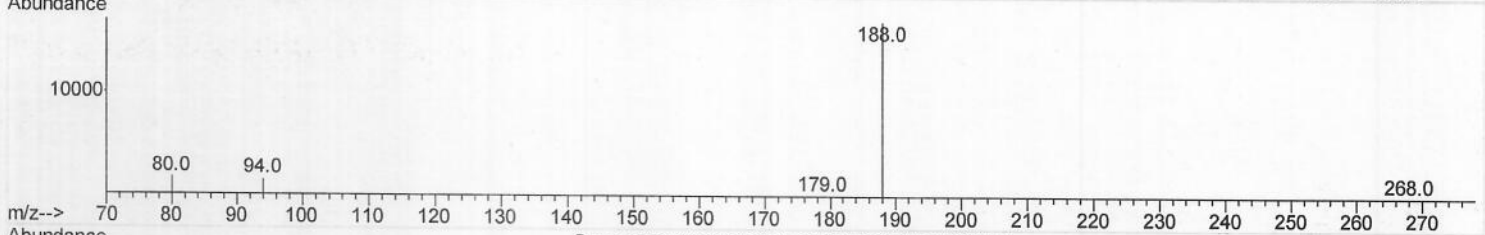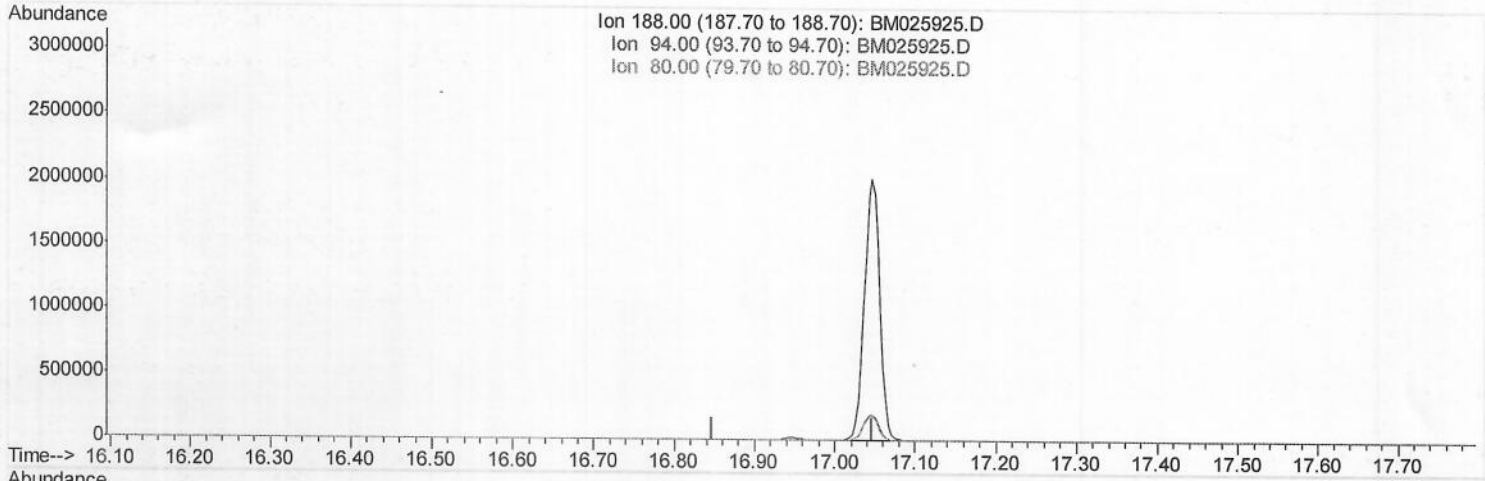

TIC: BM025925.D

(10) Phenanthrene-d10 (I)

16.947min (-16.947) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	8.20	0.00#
80.00	9.50	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM040420\
 Data File : BM025925.D
 Acq On : 03 Apr 2020 22:59
 Operator : CG/JU
 Sample : PB127888BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK88

Manual Integrations
 APPROVED

mohammad
 4/6/2020 1:41:15 PM

Quant Time: Apr 04 00:30:09 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM040220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 03 22:53:21 2020
 Response via : Initial Calibration

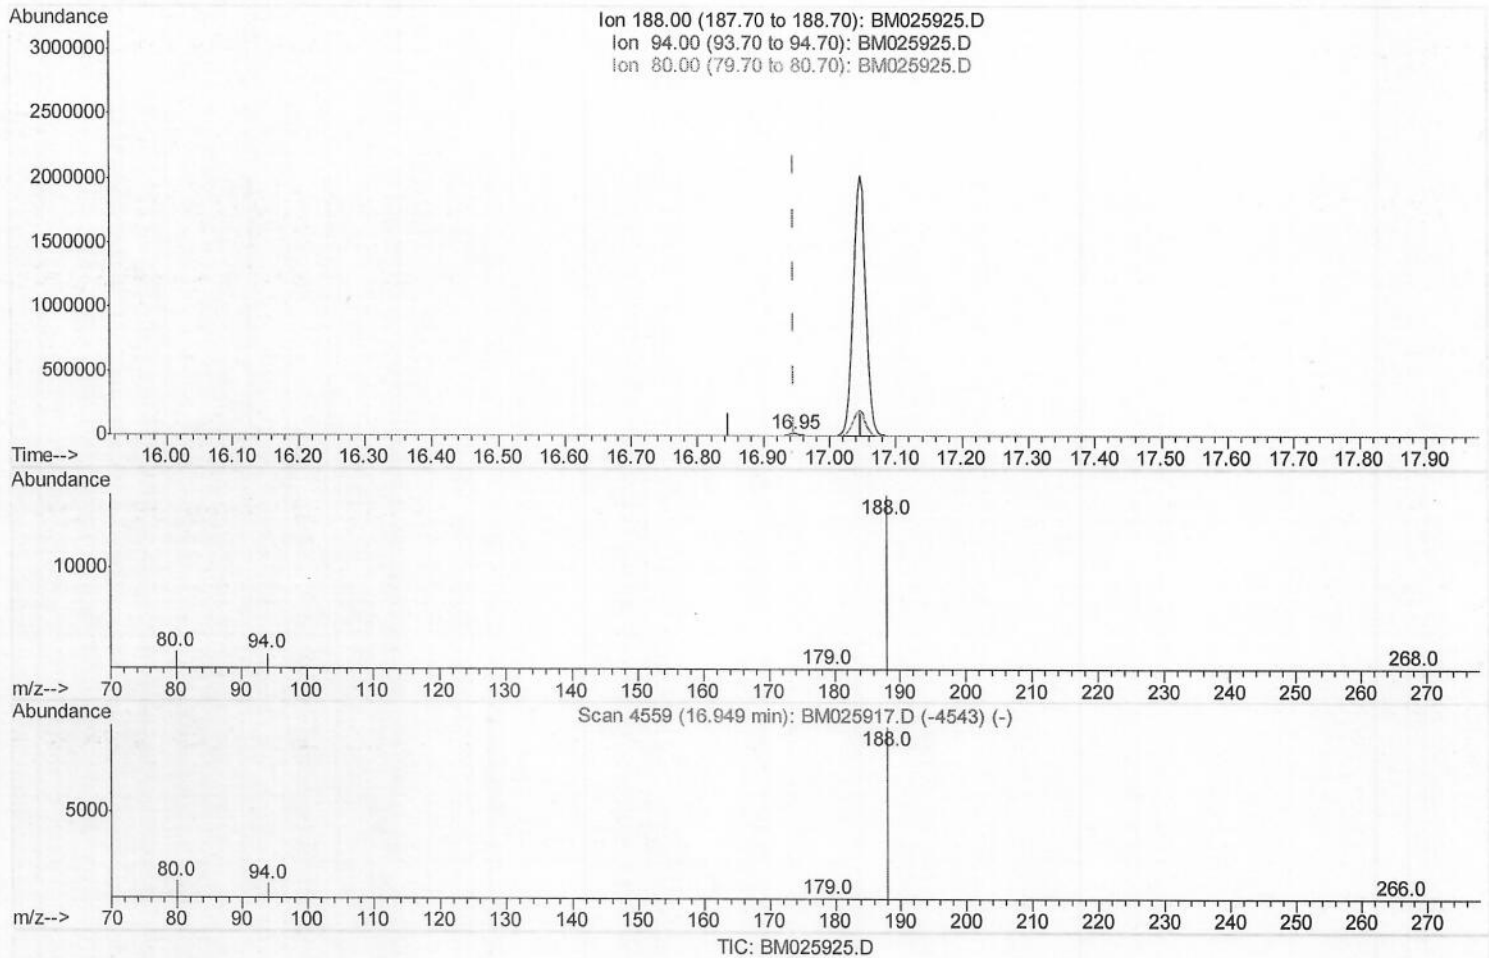

(10) Phenanthrene-d10 (I)

16.946min (-0.001) 0.40ng/ul m

response 22892

Ion	Exp%	Act%
188.00	100	100
94.00	8.20	8.82
80.00	9.50	9.85
0.00	0.00	0.00

AP
 04/8/2020

Quantitation Report (QT Reviewed)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM040420\
 Data File : BM025925.D
 Acq On : 03 Apr 2020 22:59
 Operator : CG/JU
 Sample : PB127888BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK88

Manual Integrations
 APPROVED

mohammad
 4/6/2020 1:41:15 PM

Quant Time: Apr 04 00:31:56 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM040220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 03 22:53:21 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	3106	0.40	ng/ul	0.00
2) Naphthalene-d8	10.33	136	14231	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.20	164	10407	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.95	188	22892m	0.40	ng/ul	0.00
16) Chrysene-d12	21.14	240	23489	0.40	ng/ul	0.00
20) Perylene-d12	23.28	264	21692	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	11.92	152	12323	0.49	ng/ul	0.00
14) Fluoranthene-d10	18.98	212	34354	0.48	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

AP
 04/8/2020

Quantitation Report (QT Reviewed)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM040420\
 Data File : BM025925.D
 Acq On : 03 Apr 2020 22:59
 Operator : CG/JU
 Sample : PB127888BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK88

Manual Integrations
 APPROVED

mohammad
 4/6/2020 1:41:15 PM

Quant Time: Apr 04 00:31:56 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM040220.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 03 22:53:21 2020
 Response via : Initial Calibration

