

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040424\
 Data File : BM044911.D
 Acq On : 04 Apr 2024 12:59
 Operator : MA/JU
 Sample : P1948-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AH7

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 04/04/2024
 Supervised By :mohammad ahmed 04/06/2024

Quant Time: Apr 04 13:57:37 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 03 23:34:03 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.648	152	1678	0.400	ng/u1	0.00
4) Naphthalene-d8	10.424	136	5162	0.400	ng/u1	-0.02
9) Acenaphthene-d10	14.293	164	2849	0.400	ng/u1	#-0.01
13) Phenanthrene-d10	17.052	188	6564m	0.400	ng/u1	-0.02
17) Chrysene-d12	21.278	240	6078m	0.400	ng/u1	0.00
23) Perylene-d12	23.499	264	5524m	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.218	96	9758	4.427	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.046	152	2402	0.343	ng/u1	0.00
18) Fluoranthene-d10	19.094	212	6905	0.450	ng/u1	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.256	88	1199	0.567	ng/u1	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040424\
Data File : BM044911.D
Acq On : 04 Apr 2024 12:59
Operator : MA/JU
Sample : P1948-05
Misc :
ALS Vial : 9 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0AH7

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 04/04/2024
Supervised By :mohammad ahmed 04/06/2024


Quant Time: Apr 04 13:57:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 03 23:34:03 2024
Response via : Initial Calibration

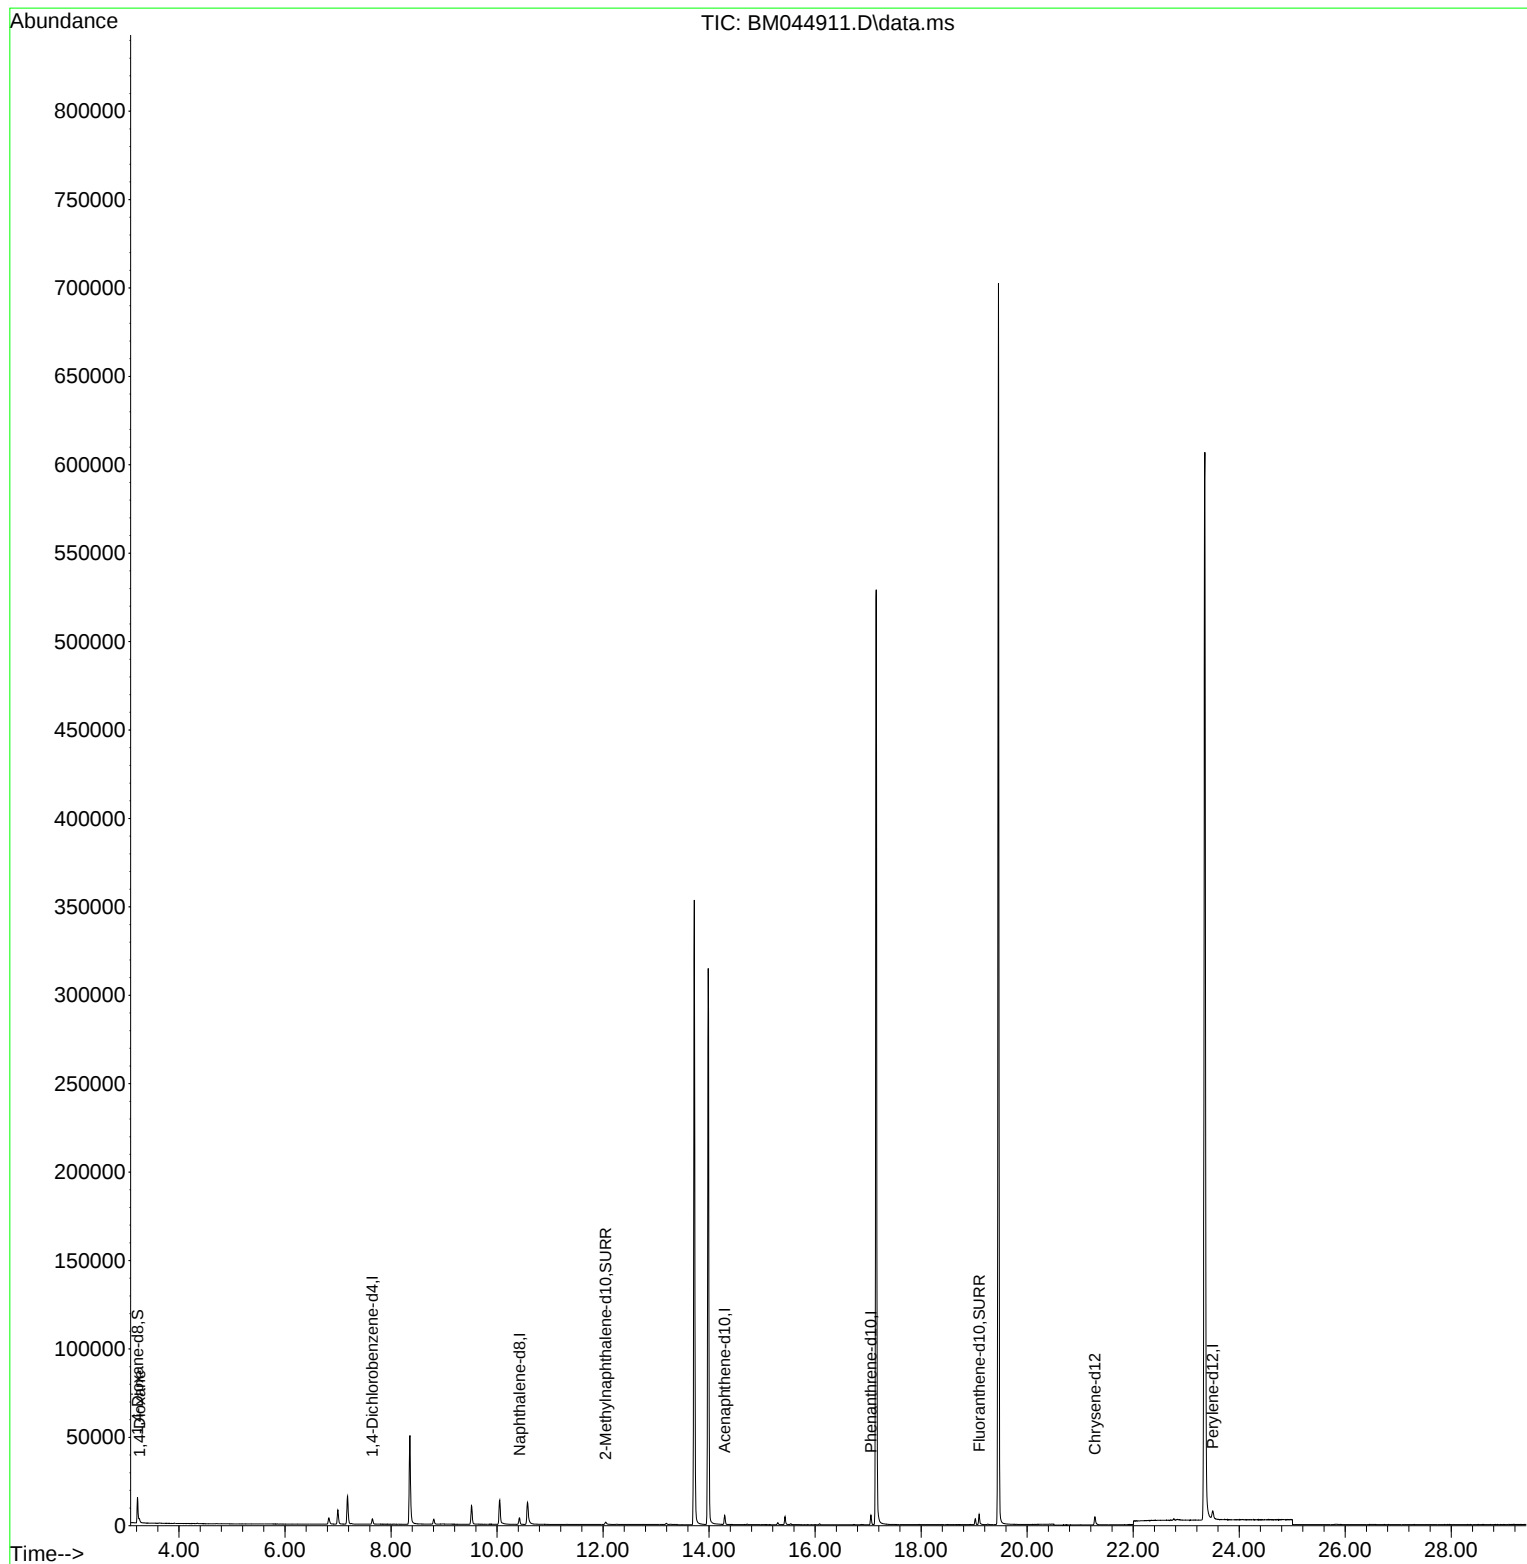

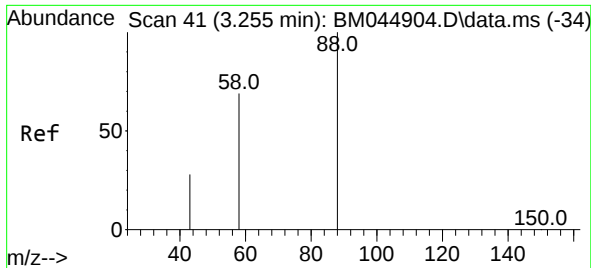

#2
 1,4-Dioxane
 Concen: 0.567 ng/ul
 RT: 3.256 min Scan# 41
 Delta R.T. 0.000 min
 Lab File: BM044911.D
 Acq: 04 Apr 2024 12:59

Instrument :
 BNA_M
 ClientSampleId :
 C0AH7

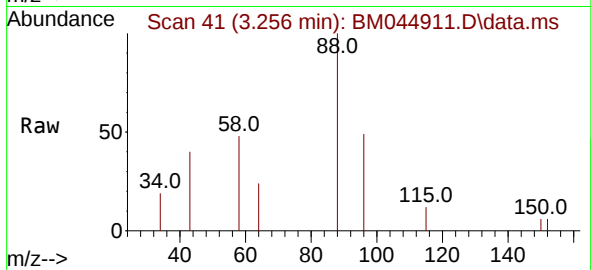

Tgt Ion: 88 Resp: 1199

Ion	Ratio	Lower	Upper
88	100		
43	39.5	30.6	46.0
58	48.2	32.6	48.8

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 04/04/2024
 Supervised By :mohammad ahmed 04/06/2024

