

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040424\
 Data File : BM044927.D
 Acq On : 04 Apr 2024 23:14
 Operator : MA/JU
 Sample : P1948-15
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AJ4

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 04/05/2024
 Supervised By :mohammad ahmed 04/06/2024

Quant Time: Apr 04 23:55:15 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 03 23:34:03 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.648	152	2201	0.400	ng/ul	0.00
4) Naphthalene-d8	10.419	136	6877	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.293	164	3771	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.052	188	8773m	0.400	ng/ul	-0.02
17) Chrysene-d12	21.263	240	7989m	0.400	ng/ul	0.00
23) Perylene-d12	23.490	264	8695m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.218	96	11300	3.908	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.024	152	3047	0.327	ng/ul	-0.03
18) Fluoranthene-d10	19.089	212	8415	0.417	ng/ul	-0.01
Target Compounds						Qvalue
2) 1,4-Dioxane	3.247	88	254205	91.718	ng/ul#	72

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040424\
Data File : BM044927.D
Acq On : 04 Apr 2024 23:14
Operator : MA/JU
Sample : P1948-15
Misc :
ALS Vial : 25 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0AJ4

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 04/05/2024
Supervised By :mohammad ahmed 04/06/2024


Quant Time: Apr 04 23:55:15 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM040424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 03 23:34:03 2024
Response via : Initial Calibration

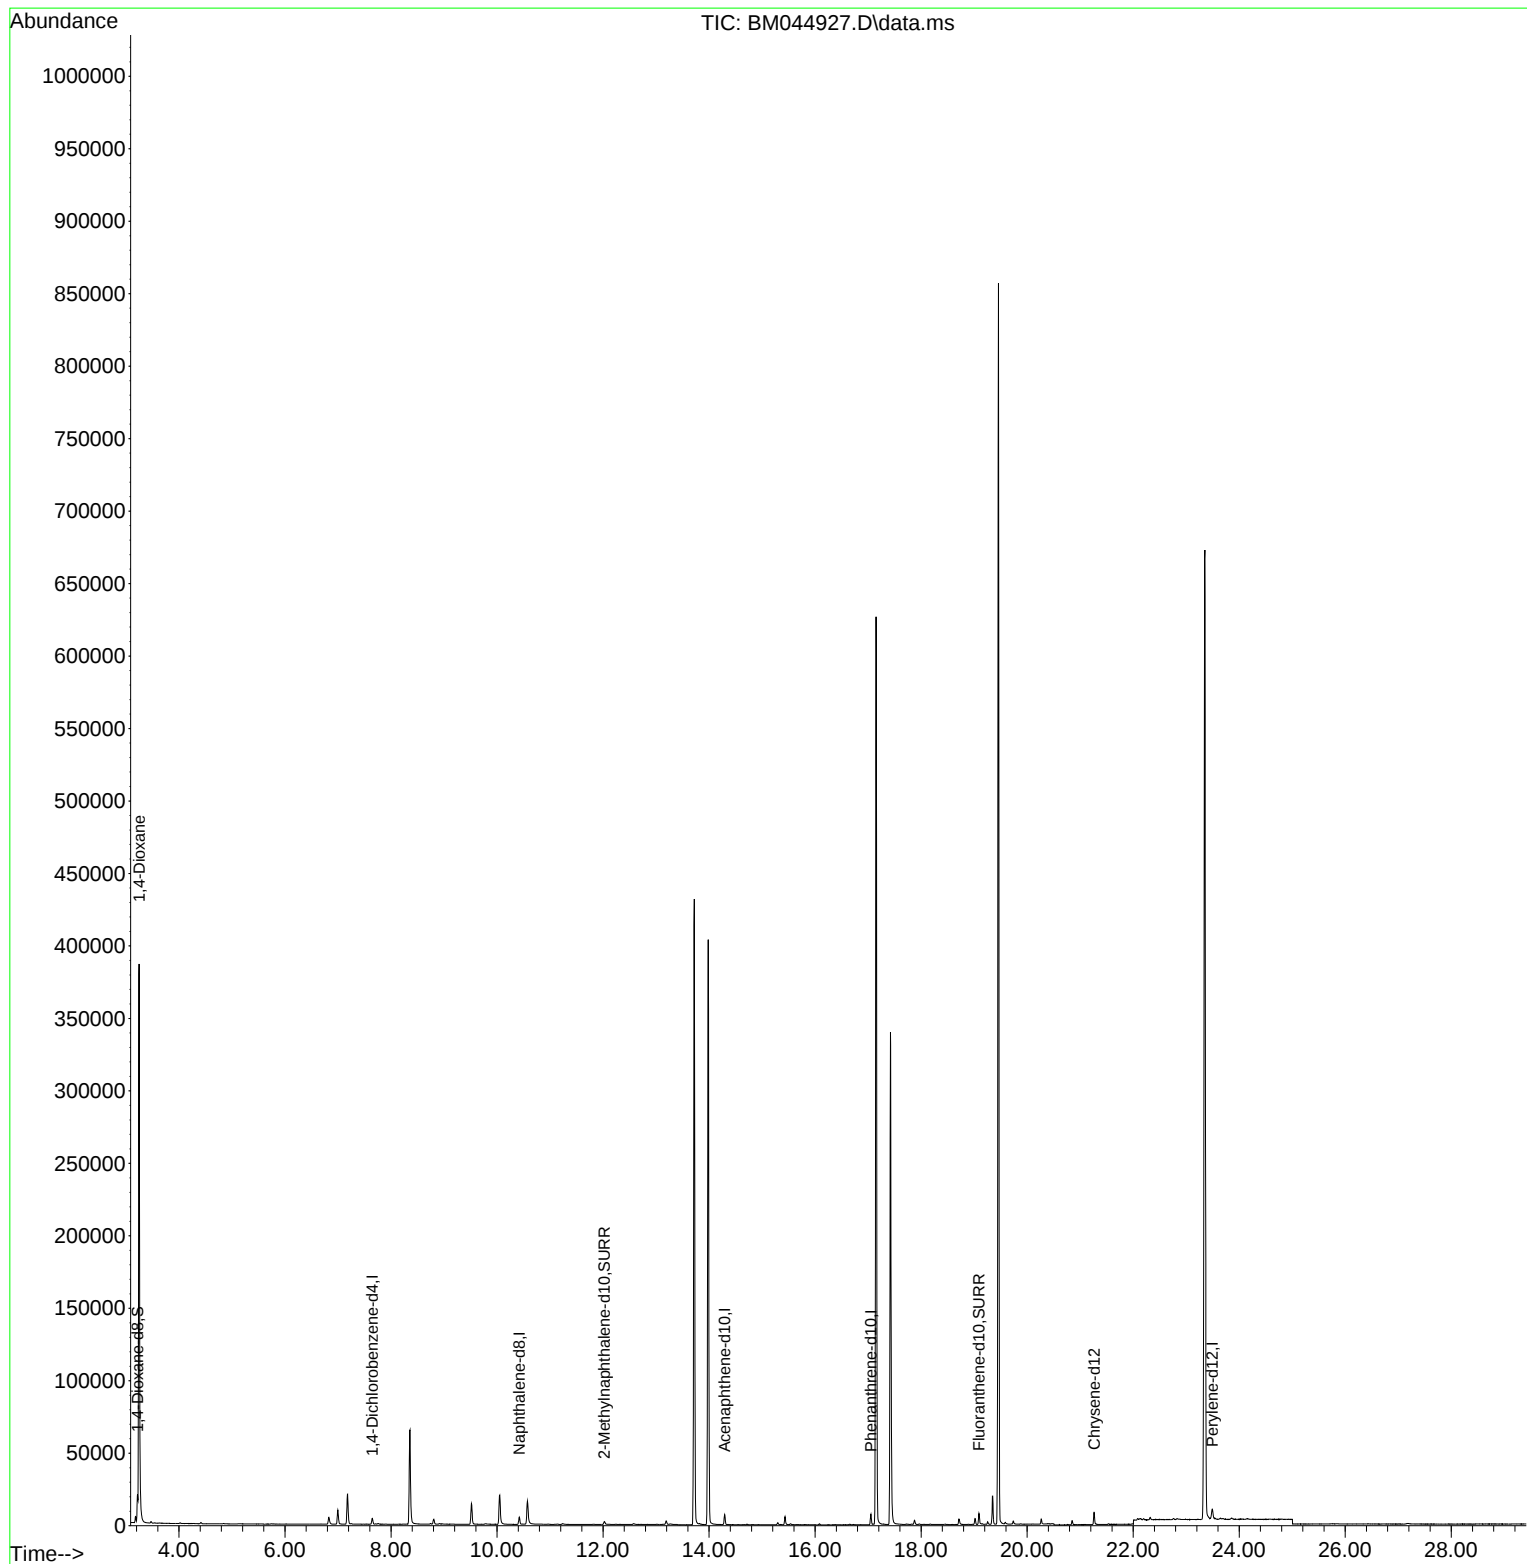

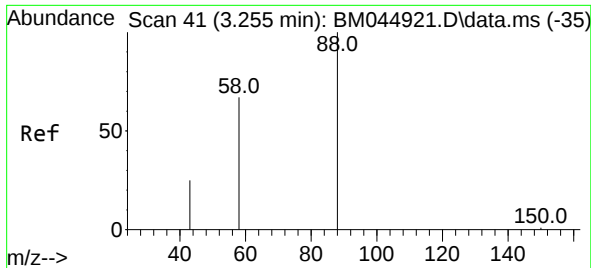

#2
1,4-Dioxane
Concen: 91.718 ng/ul
RT: 3.247 min Scan# 39
Delta R.T. -0.008 min
Lab File: BM044927.D
Acq: 04 Apr 2024 23:14

Instrument :
BNA_M
ClientSampleId :
C0AJ4

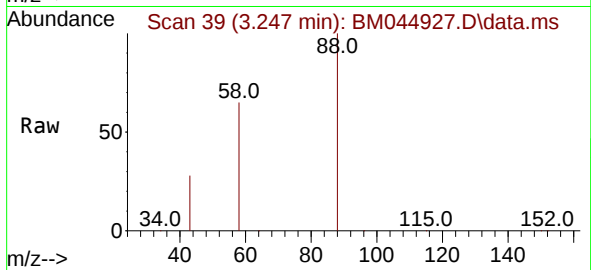

Tgt Ion: 88 Resp: 25420
Ion Ratio Lower Upper
88 100
43 27.9 30.6 46.0
58 64.7 32.6 48.8

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 04/05/2024
Supervised By :mohammad ahmed 04/06/2024

