




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040522\
 Data File : BM034497.D
 Acq On : 05 Apr 2022 10:44
 Operator : CG/JU
 Sample : PB143816BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK816

Manual IntegrationsAPPROVED

Quant Time: Apr 06 05:40:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 11:50:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/06/2022
 Supervised By :Yogesh Patel 04/09/2022

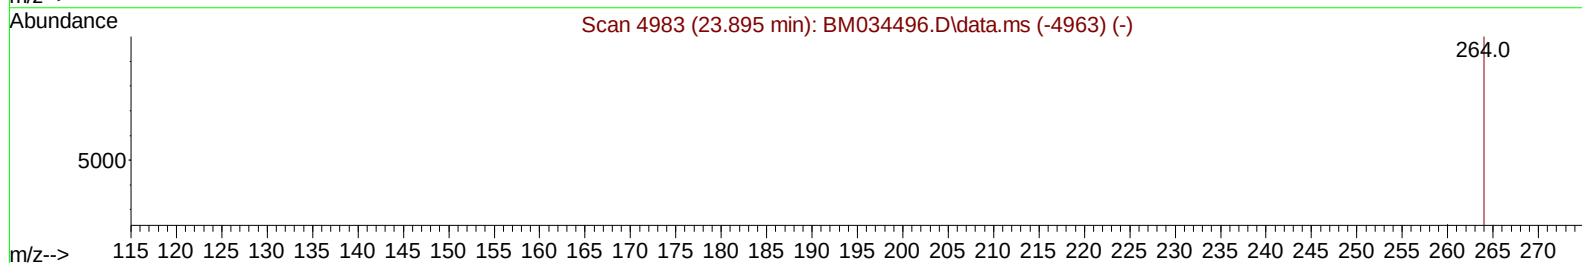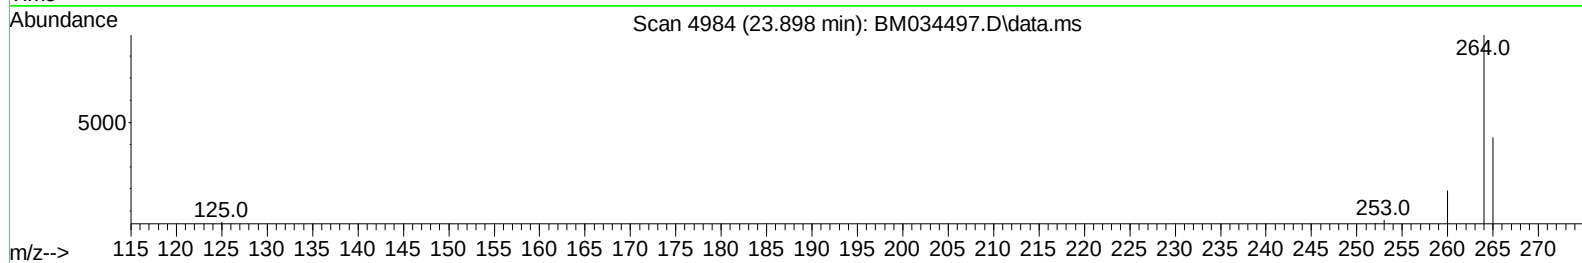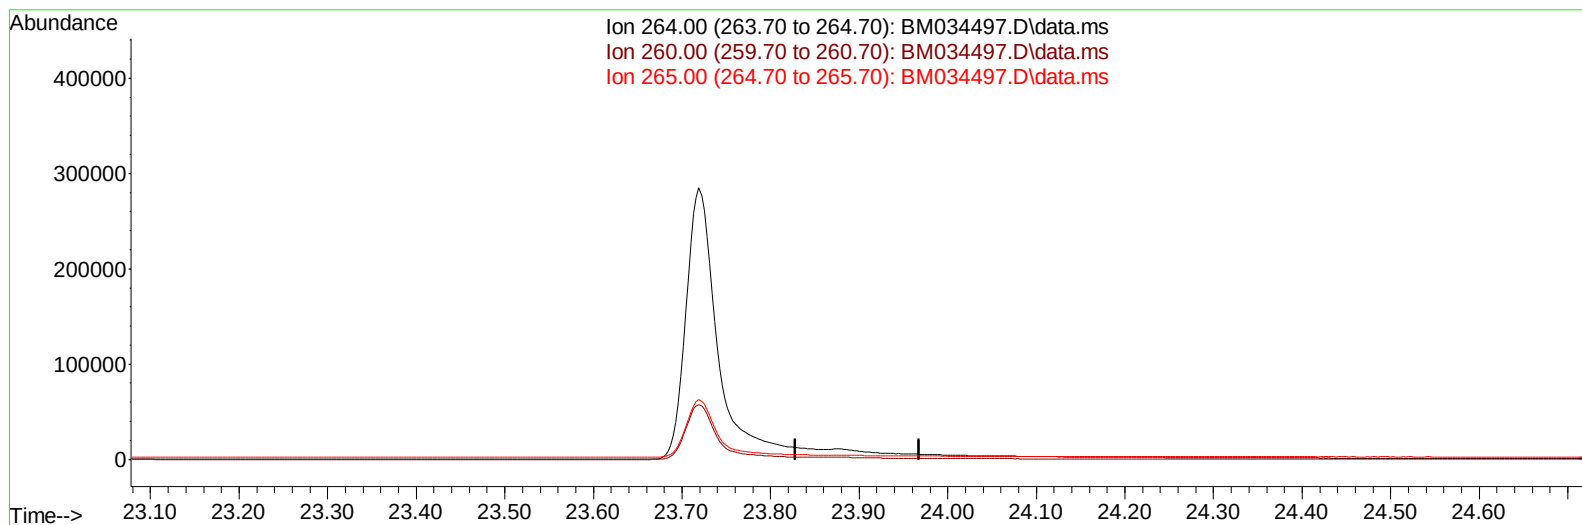

TIC: BM034497.D\data.ms

(23) Perylene-d12 (I)

23.898min (-23.898) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	27.80	0.00#
265.00	95.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040522\
 Data File : BM034497.D
 Acq On : 05 Apr 2022 10:44
 Operator : CG/JU
 Sample : PB143816BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK816

Manual IntegrationsAPPROVED

Quant Time: Apr 06 05:40:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 11:50:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/06/2022
 Supervised By :Yogesh Patel 04/09/2022

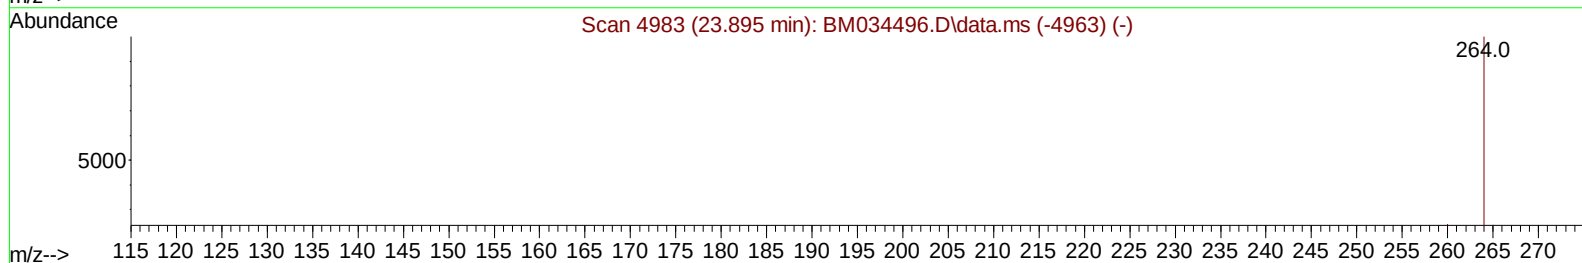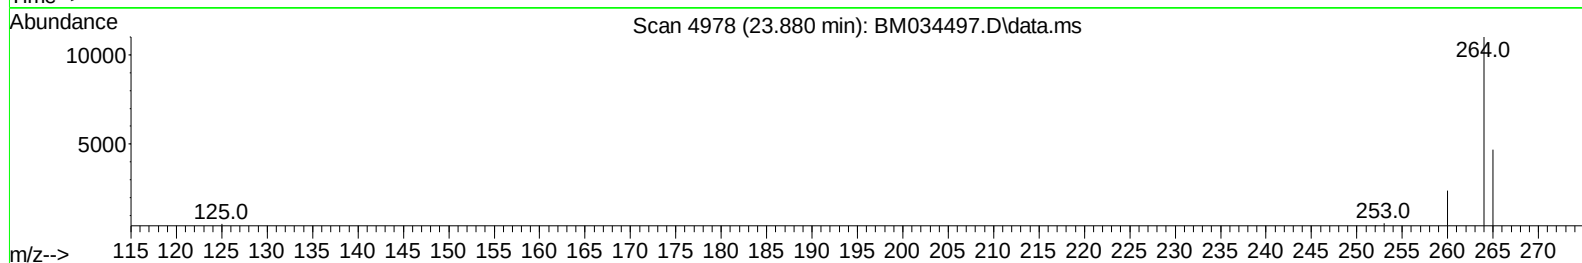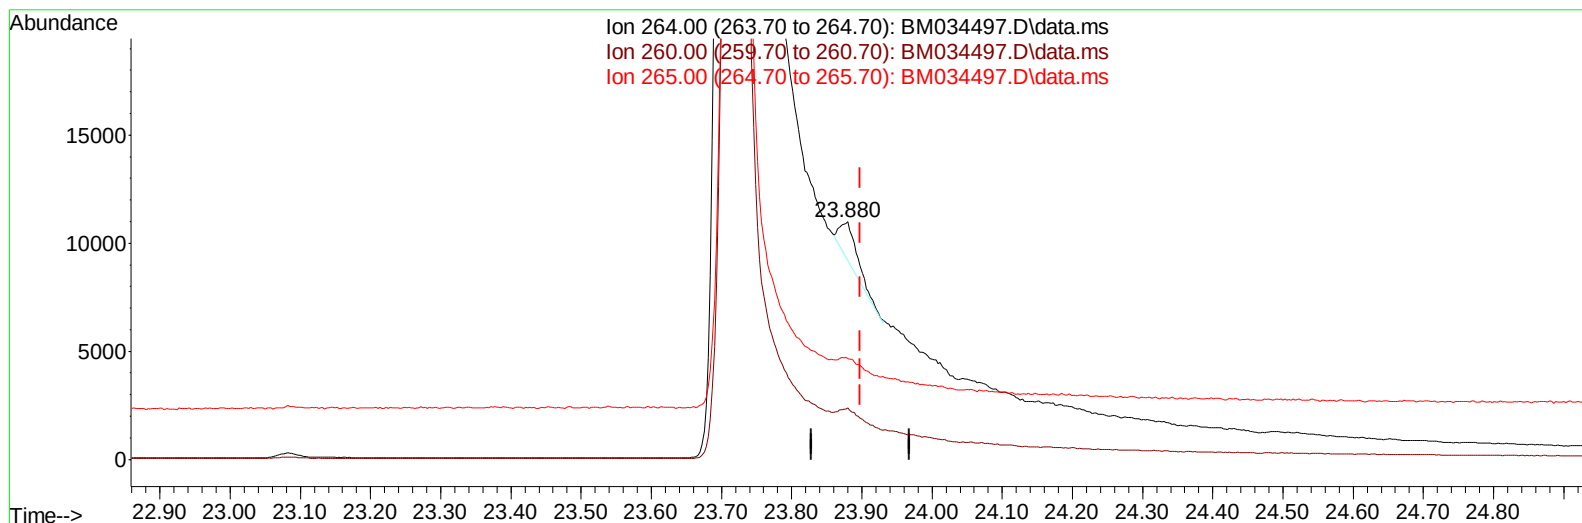

TIC: BM034497.D\data.ms

(23) Perylene-d12 (I)

23.880min (-0.018) 0.40 ng/ul m

response 2693

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.80	21.65#
265.00	95.30	42.40#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040522\
 Data File : BM034497.D
 Acq On : 05 Apr 2022 10:44
 Operator : CG/JU
 Sample : PB143816BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK816

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/06/2022
 Supervised By :Yogesh Patel 04/09/2022

Quant Time: Apr 06 05:40:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 11:50:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.912	152	2915	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.724	136	7785	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.555	164	4182	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.299	188	7527	0.400	ng/ul	-0.01
17) Chrysene-d12	21.518	240	5595	0.400	ng/ul	# 0.02
23) Perylene-d12	23.880	264	2693m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.292	96	28929	5.925	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.341	152	3943	0.386	ng/ul	0.00
18) Fluoranthene-d10	19.329	212	7460	0.454	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040522\
Data File : BM034497.D
Acq On : 05 Apr 2022 10:44
Operator : CG/JU
Sample : PB143816BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK816

Manual IntegrationsAPPROVED

Quant Time: Apr 06 05:40:34 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 05 11:50:53 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/06/2022
Supervised By :Yogesh Patel 04/09/2022

