




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040522\
 Data File : BM034499.D
 Acq On : 05 Apr 2022 13:09
 Operator : CG/JU
 Sample : N2166-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0R39

Manual IntegrationsAPPROVED

Quant Time: Apr 06 01:16:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 11:50:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/06/2022
 Supervised By :Yogesh Patel 04/09/2022

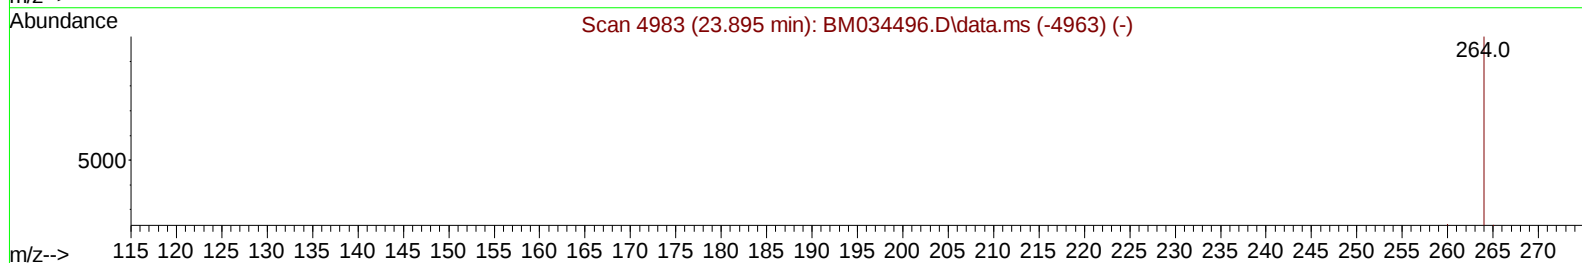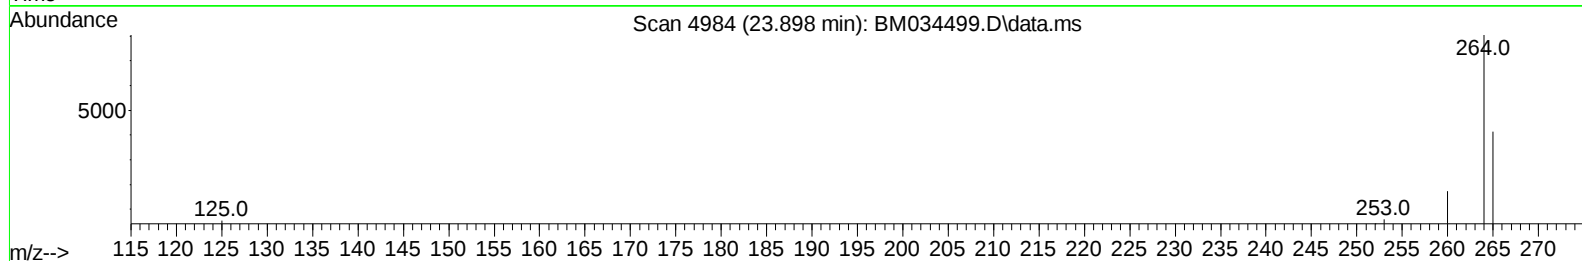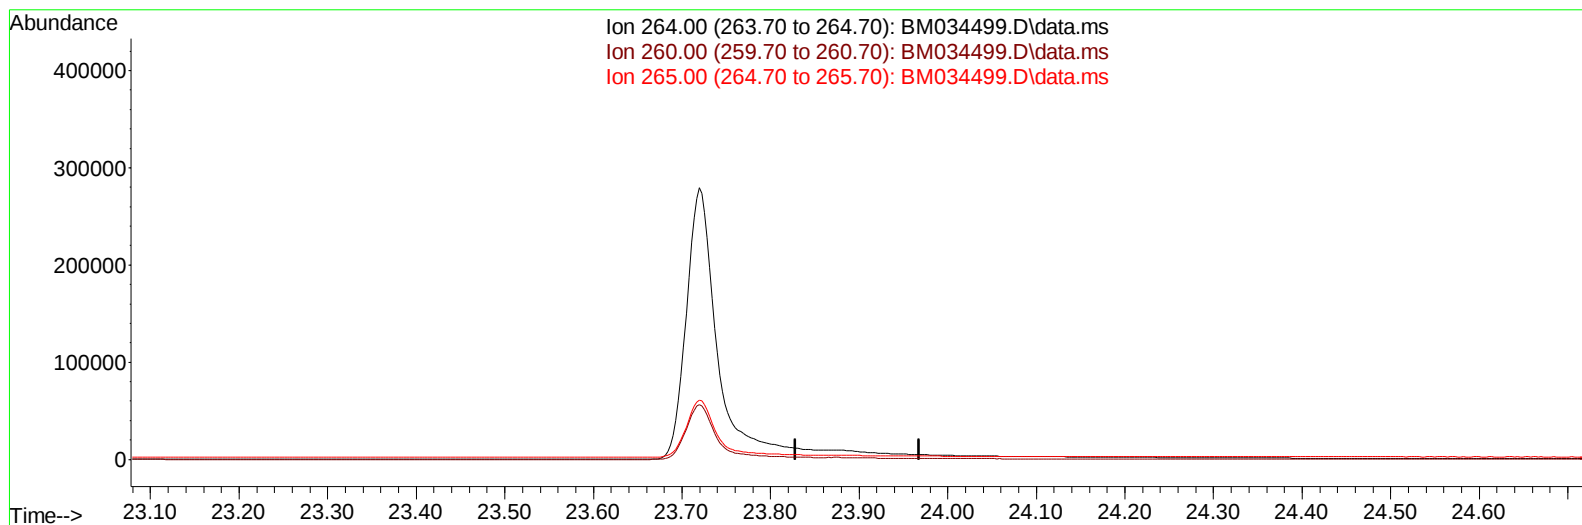

TIC: BM034499.D\data.ms

(23) Perylene-d12 (I)

23.898min (-23.898) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	27.80	0.00#
265.00	95.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040522\
 Data File : BM034499.D
 Acq On : 05 Apr 2022 13:09
 Operator : CG/JU
 Sample : N2166-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0R39

Manual IntegrationsAPPROVED

Quant Time: Apr 06 01:16:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 11:50:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/06/2022
 Supervised By :Yogesh Patel 04/09/2022

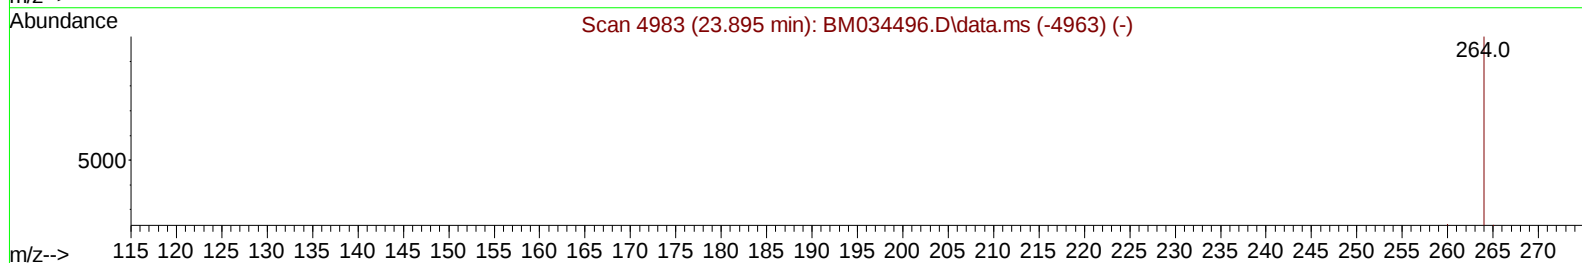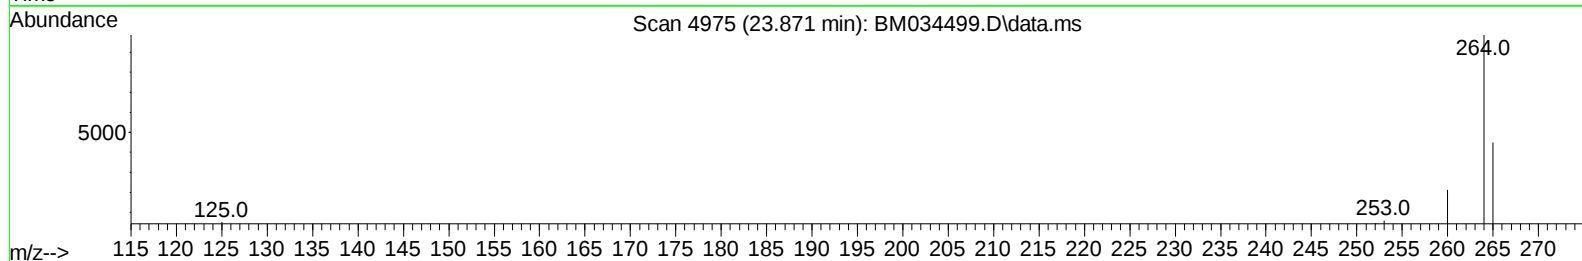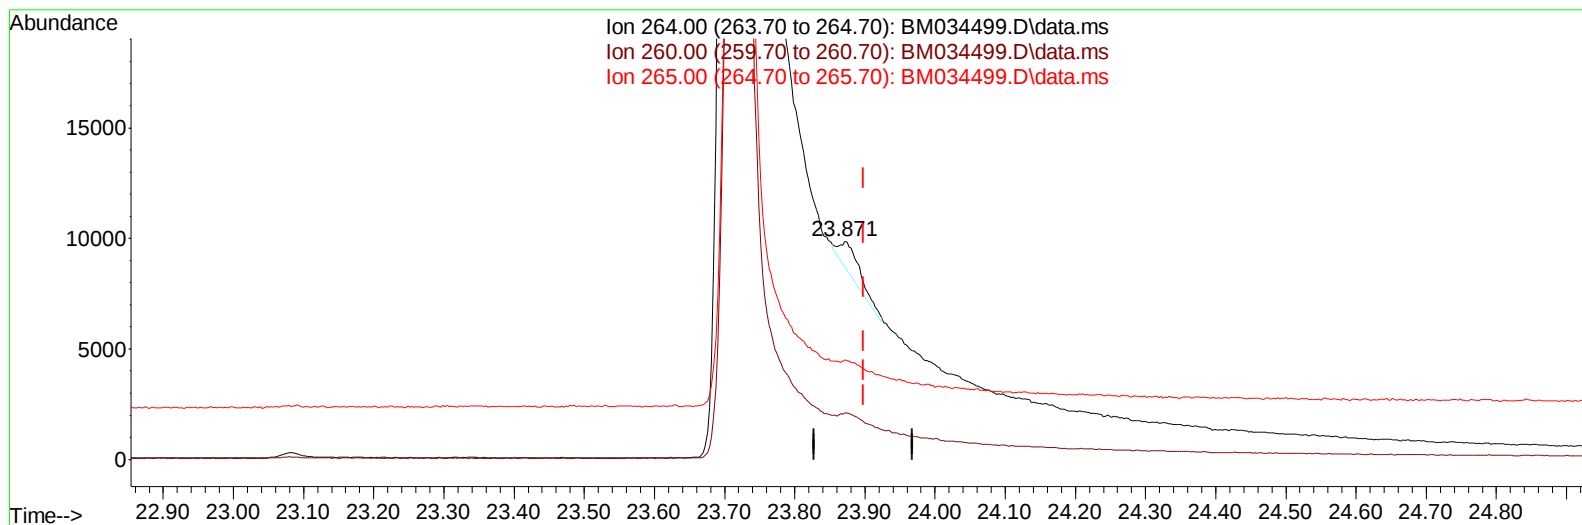

TIC: BM034499.D\data.ms

(23) Perylene-d12 (I)

23.871min (-0.027) 0.40 ng/ul m

response 2531

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.80	21.41#
265.00	95.30	45.55#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040522\
 Data File : BM034499.D
 Acq On : 05 Apr 2022 13:09
 Operator : CG/JU
 Sample : N2166-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0R39

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/06/2022
 Supervised By :Yogesh Patel 04/09/2022

Quant Time: Apr 06 01:16:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 11:50:53 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.916	152		2521	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.724	136		6953	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.555	164		3783	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.299	188		6800	0.400	ng/ul	-0.01
17) Chrysene-d12	21.518	240		4704	0.400	ng/ul	# 0.02
23) Perylene-d12	23.871	264		2531m	0.400	ng/ul	-0.03
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.292	96		21439	5.077	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.330	152		3684	0.404	ng/ul	0.00
18) Fluoranthene-d10	19.329	212		7938	0.575	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040522\
Data File : BM034499.D
Acq On : 05 Apr 2022 13:09
Operator : CG/JU
Sample : N2166-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0R39

Manual IntegrationsAPPROVED

Quant Time: Apr 06 01:16:28 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 05 11:50:53 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/06/2022
Supervised By :Yogesh Patel 04/09/2022

