




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040522\
 Data File : BM034500.D
 Acq On : 05 Apr 2022 13:45
 Operator : CG/JU
 Sample : N2166-04
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0R40

Manual IntegrationsAPPROVED

Quant Time: Apr 06 01:22:25 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 11:50:53 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/06/2022
 Supervised By :Yogesh Patel 04/09/2022

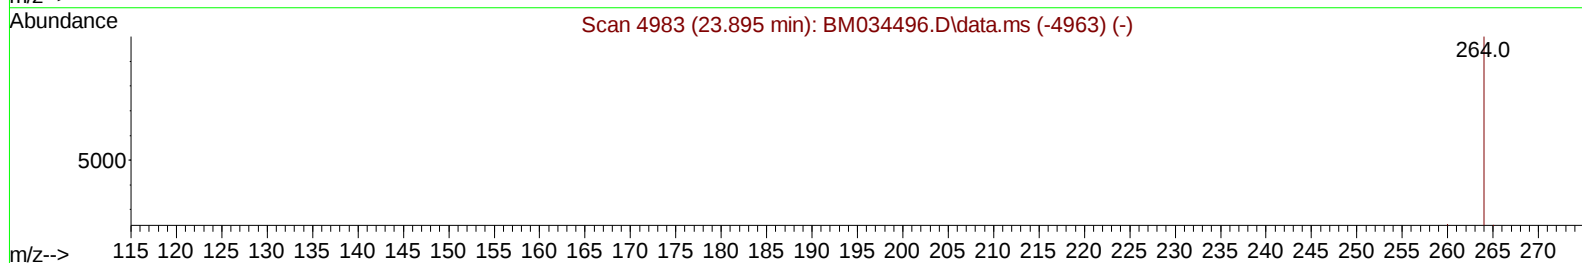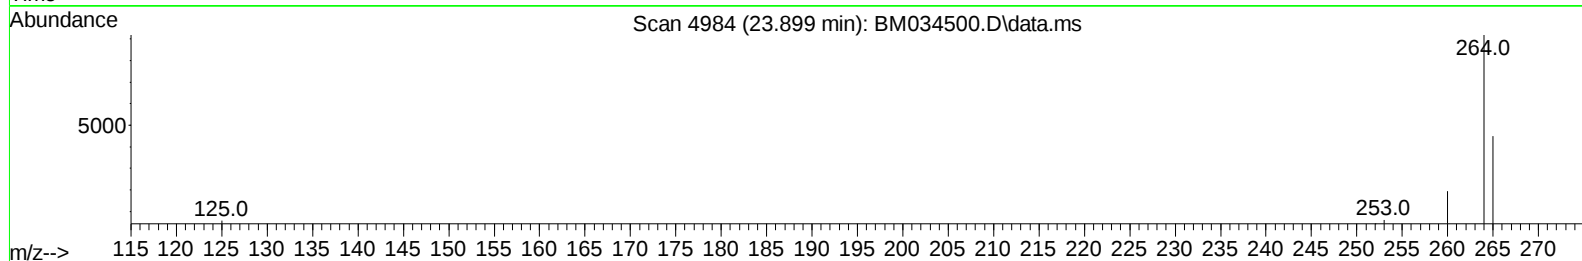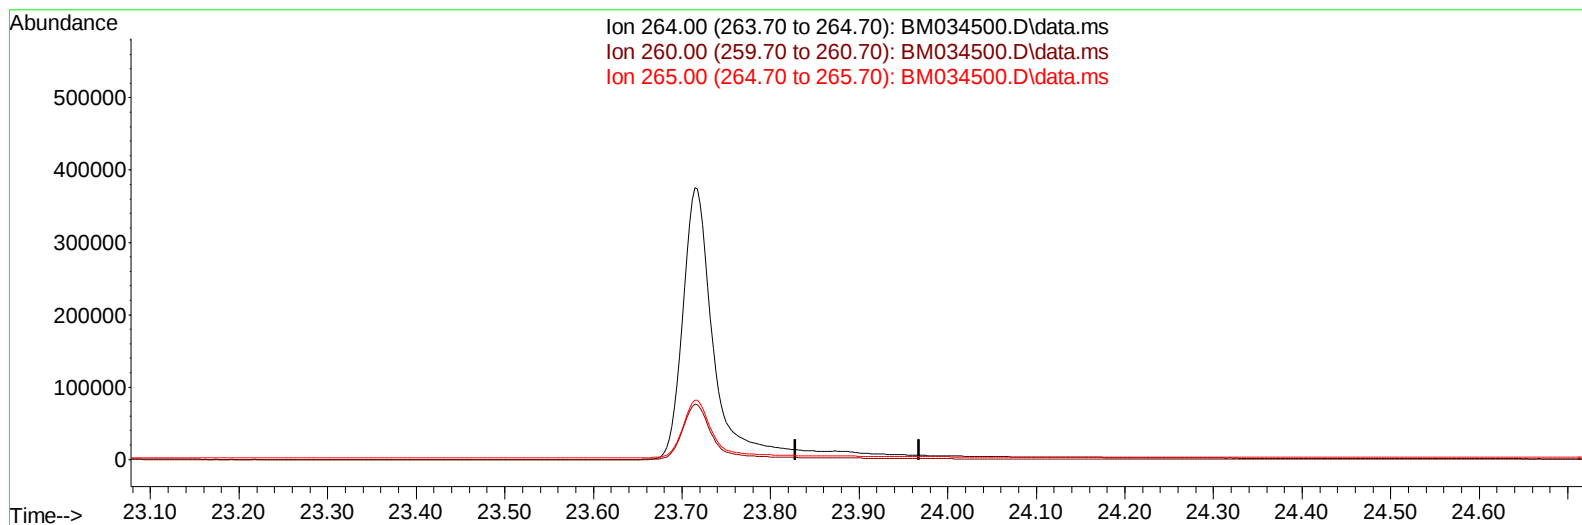

TIC: BM034500.D\data.ms

(23) Perylene-d12 (I)

23.898min (-23.898) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	27.80	0.00#
265.00	95.30	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040522\
Data File : BM034500.D
Acq On : 05 Apr 2022 13:45
Operator : CG/JU
Sample : N2166-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0R40

Manual IntegrationsAPPROVED

Quant Time: Apr 06 01:22:25 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 05 11:50:53 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/06/2022
Supervised By :Yogesh Patel 04/09/2022

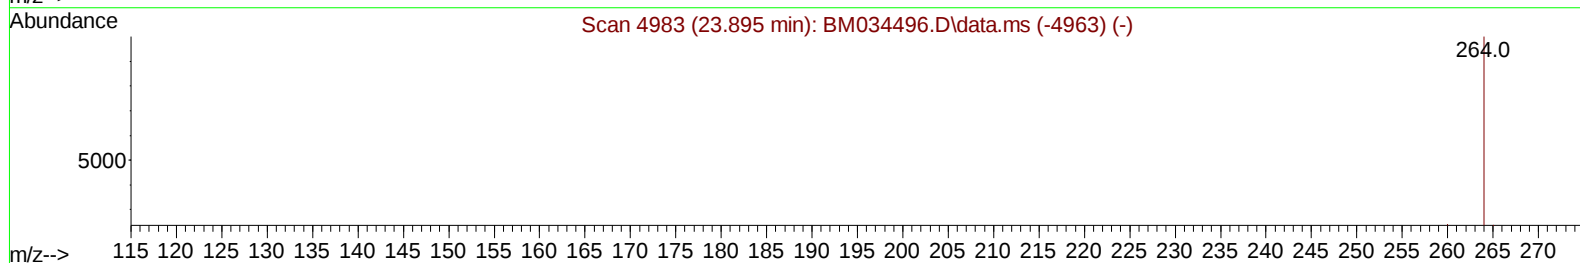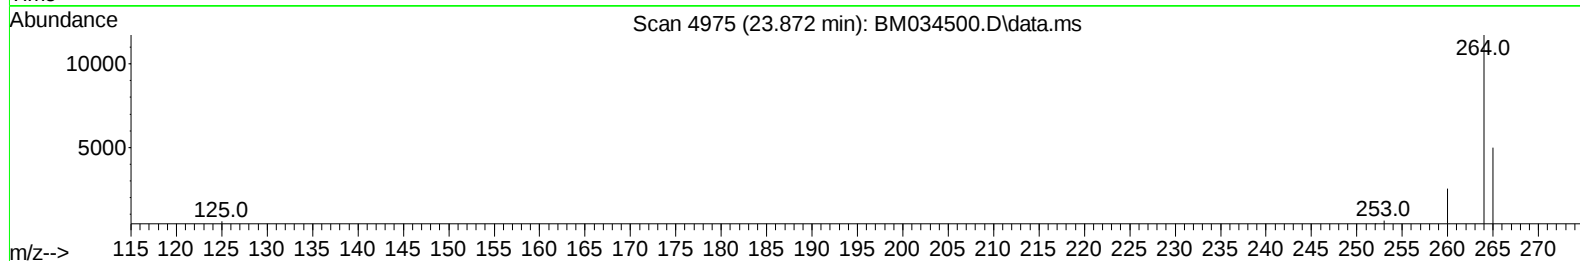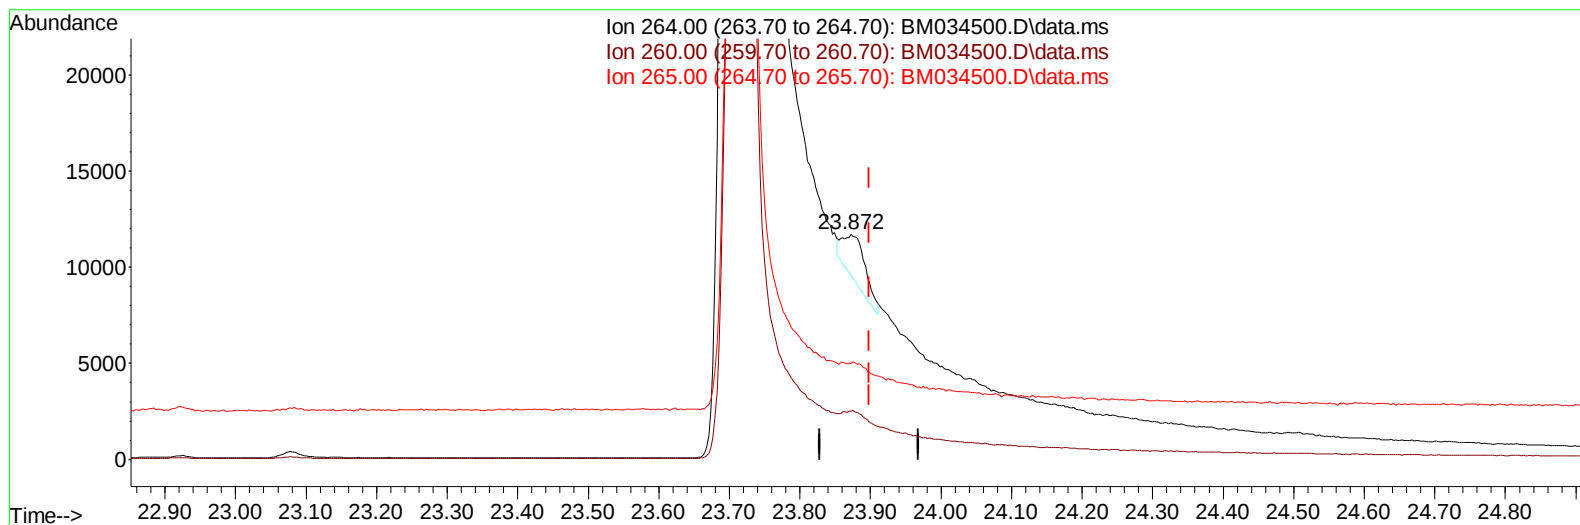

TIC: BM034500.D\data.ms

(23) Perylene-d12 (I)

23.872min (-0.026) 0.40 ng/ul m

response 5065

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.80	21.55#
265.00	95.30	42.60#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040522\
 Data File : BM034500.D
 Acq On : 05 Apr 2022 13:45
 Operator : CG/JU
 Sample : N2166-04
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0R40

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 04/06/2022
 Supervised By :Yogesh Patel 04/09/2022

Quant Time: Apr 06 01:22:25 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 11:50:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.912	152	3111	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.720	136	8288	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.556	164	4720	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.296	188	9139	0.400	ng/ul	-0.02
17) Chrysene-d12	21.514	240	7230	0.400	ng/ul	# 0.02
23) Perylene-d12	23.872	264	5065m	0.400	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	24063	4.618	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.320	152	3983	0.366	ng/ul	-0.01
18) Fluoranthene-d10	19.326	212	10159	0.479	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040522\
Data File : BM034500.D
Acq On : 05 Apr 2022 13:45
Operator : CG/JU
Sample : N2166-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0R40

Manual IntegrationsAPPROVED

Quant Time: Apr 06 01:22:25 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 05 11:50:53 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 04/06/2022
Supervised By :Yogesh Patel 04/09/2022

