

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
 Data File : BM044983.D
 Acq On : 06 Apr 2024 23:15
 Operator : MA/JU
 Sample : P2012-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Apr 08 05:05:02 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 08 05:01:54 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.634	152	73885	20.000	ng/ul	0.00
20) Naphthalene-d8	10.410	136	328631	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.280	164	211012	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.039	188	451897	20.000	ng/ul	0.00
79) Chrysene-d12	21.250	240	461730	20.000	ng/ul	0.00
88) Perylene-d12	23.474	264	557041	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.210	96	9301	4.701	ng/uL	0.00
4) Pyridine-d5	3.622	84	38453	7.147	ng/ul	0.01
7) Phenol-d5	6.816	99	44093	7.040	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.987	67	140951	37.770	ng/ul	0.00
11) 2-Chlorophenol-d4	7.169	132	146801	29.915	ng/ul	0.00
15) 4-Methylphenol-d8	8.345	113	89301	18.214	ng/ul	0.00
21) Nitrobenzene-d5	8.798	128	95591	37.868	ng/ul	0.00
24) 2-Nitrophenol-d4	9.504	143	104177	39.100	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.039	165	168381	34.469	ng/ul	0.00
31) 4-Chloroaniline-d4	10.563	131	227682	29.274	ng/ul	0.00
46) Dimethylphthalate-d6	13.710	166	621178	42.279	ng/ul	0.00
49) Acenaphthylene-d8	13.974	160	706982	40.732	ng/ul	0.00
54) 4-Nitrophenol-d4	14.539	143	13646	4.450	ng/ul	0.02
60) Fluorene-d10	15.280	176	568516	43.403	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.427	200	96409	35.982	ng/ul	0.00
73) Anthracene-d10	17.139	188	960631	47.255	ng/ul	0.00
81) Pyrene-d10	19.445	212	1172105	51.554	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.333	264	1322240	48.658	ng/ul	0.00


Target Compounds					Qvalue	
2) 1,4-Dioxane	3.246	88	6931	3.354	ng/uL#	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM044983.D
Acq On : 06 Apr 2024 23:15
Operator : MA/JU
Sample : P2012-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :


Quant Time: Apr 08 05:05:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 08 05:01:54 2024
Response via : Initial Calibration

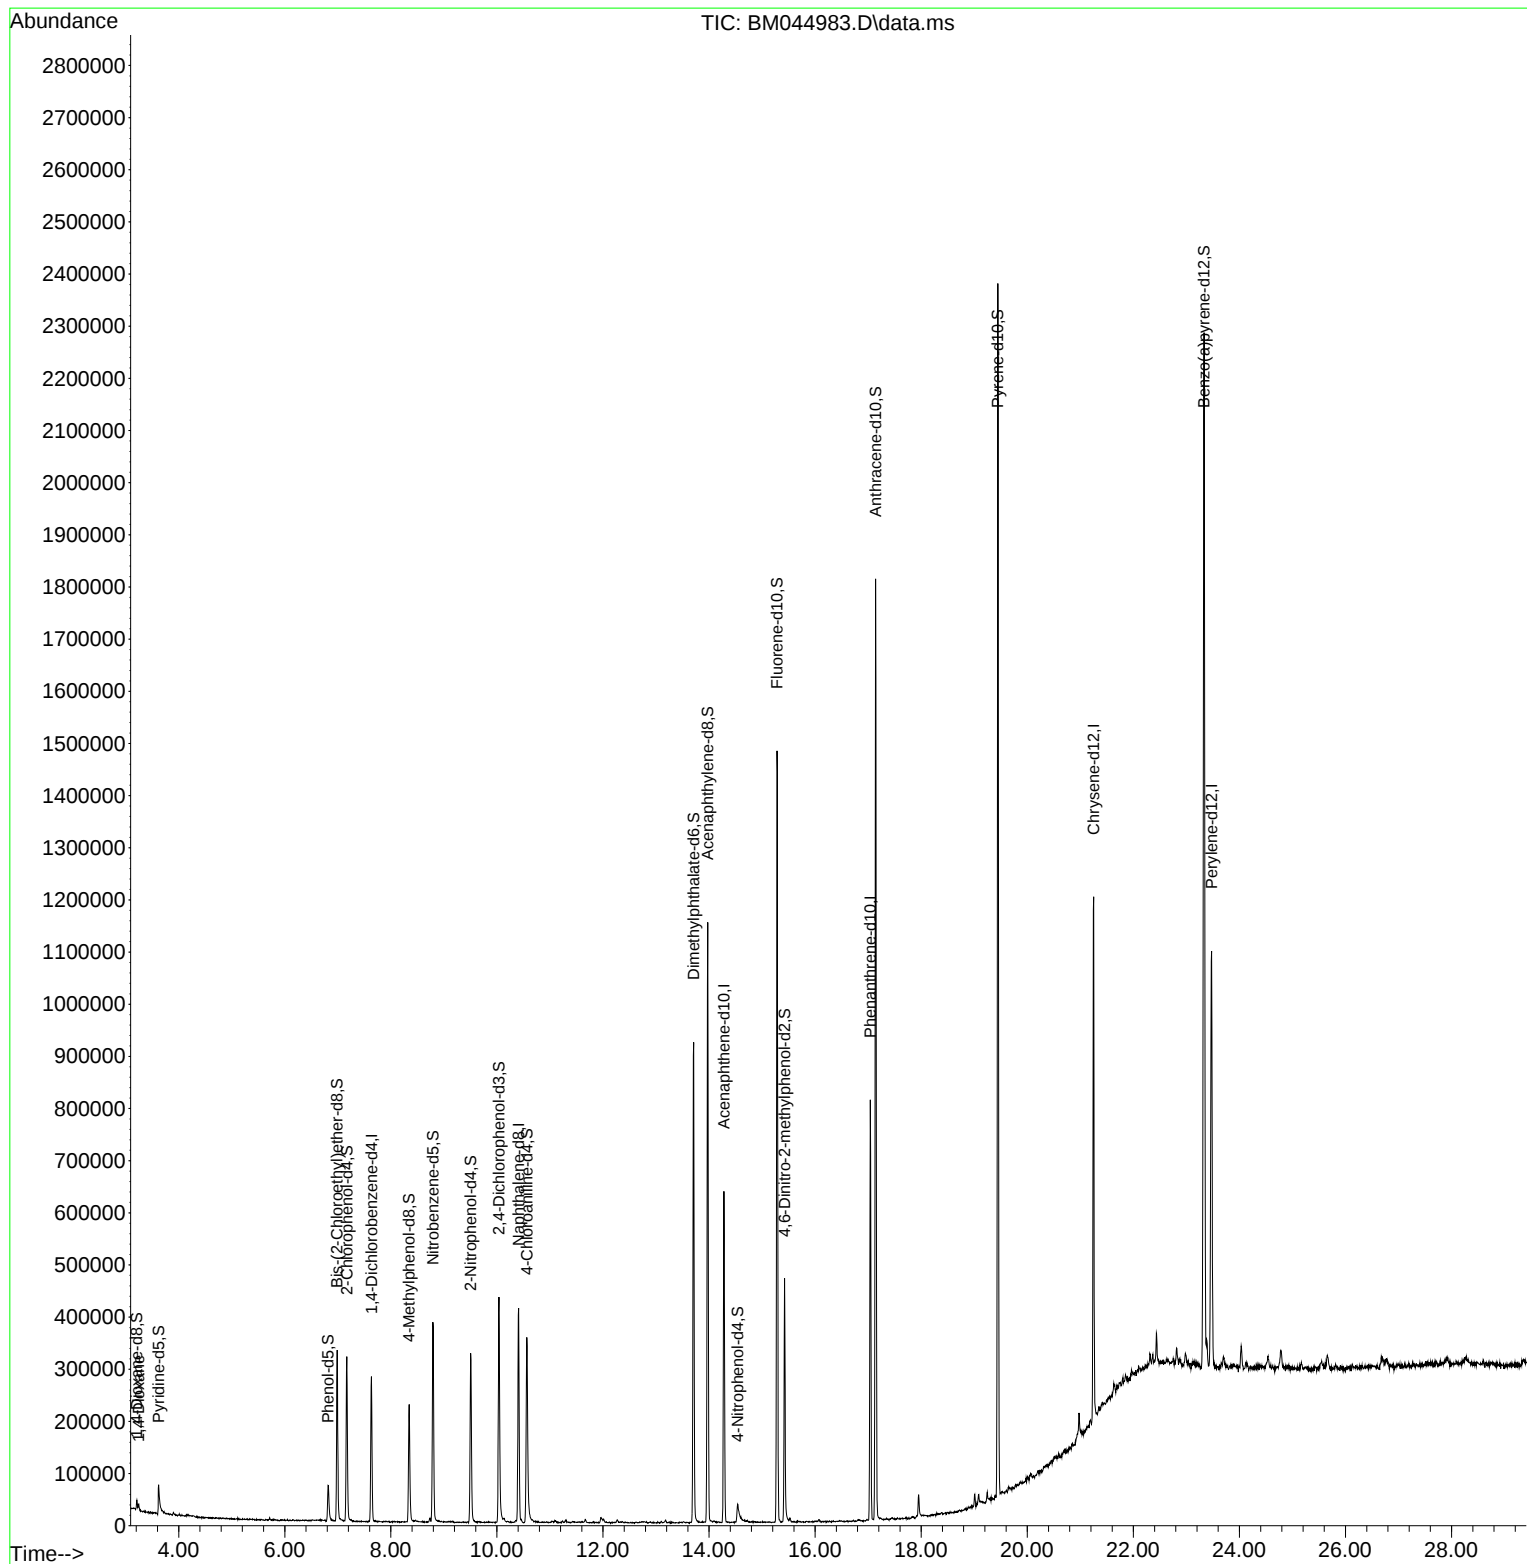

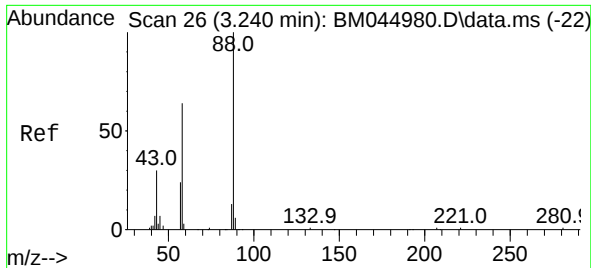

#2
 1,4-Dioxane
 Concen: 3.354 ng/uL
 RT: 3.246 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: BM044983.D
 Acq: 06 Apr 2024 23:15

Instrument :
 BNA_M
 ClientSampleId :

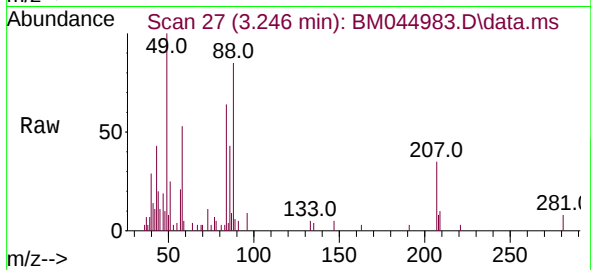

Tgt Ion: 88 Resp: 6931
 Ion Ratio Lower Upper
 88 100
 43 50.9 24.0 36.0#
 58 62.7 45.4 68.2

