

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
 Data File : BM044998.D
 Acq On : 07 Apr 2024 08:48
 Operator : MA/JU
 Sample : PB160055BL
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Apr 08 05:53:41 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 08 05:51:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.628	152	65409	20.000	ng/ul	0.00
20) Naphthalene-d8	10.404	136	294599	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.280	164	187067	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.039	188	388980	20.000	ng/ul	0.00
79) Chrysene-d12	21.244	240	350960	20.000	ng/ul	0.00
88) Perylene-d12	23.468	264	426089	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.210	96	11045	6.306	ng/uL	0.00
4) Pyridine-d5	3.604	84	172053	36.120	ng/ul	0.00
7) Phenol-d5	6.816	99	209513	37.784	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.987	67	124255	37.611	ng/ul	0.00
11) 2-Chlorophenol-d4	7.163	132	171674	39.517	ng/ul	0.00
15) 4-Methylphenol-d8	8.339	113	168892	38.912	ng/ul	0.00
21) Nitrobenzene-d5	8.792	128	82163	36.309	ng/ul	0.00
24) 2-Nitrophenol-d4	9.504	143	91013	38.105	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.033	165	161621	36.907	ng/ul	0.00
31) 4-Chloroaniline-d4	10.563	131	275714	39.545	ng/ul	0.00
46) Dimethylphthalate-d6	13.704	166	468366	35.959	ng/ul	0.00
49) Acenaphthylene-d8	13.968	160	566434	36.812	ng/ul	0.00
54) 4-Nitrophenol-d4	14.521	143	74353	27.353	ng/ul	0.00
60) Fluorene-d10	15.280	176	423478	36.469	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.421	200	53127	23.035	ng/ul	0.00
73) Anthracene-d10	17.139	188	671674	38.385	ng/ul	0.00
81) Pyrene-d10	19.445	212	762771	44.139	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.327	264	822510	39.571	ng/ul	0.00


Target Compounds					Qvalue	
17) N-Nitroso-di-n-propyla...	8.339	70	4753	1.427	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM044998.D
Acq On : 07 Apr 2024 08:48
Operator : MA/JU
Sample : PB160055BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :


Quant Time: Apr 08 05:53:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 08 05:51:38 2024
Response via : Initial Calibration

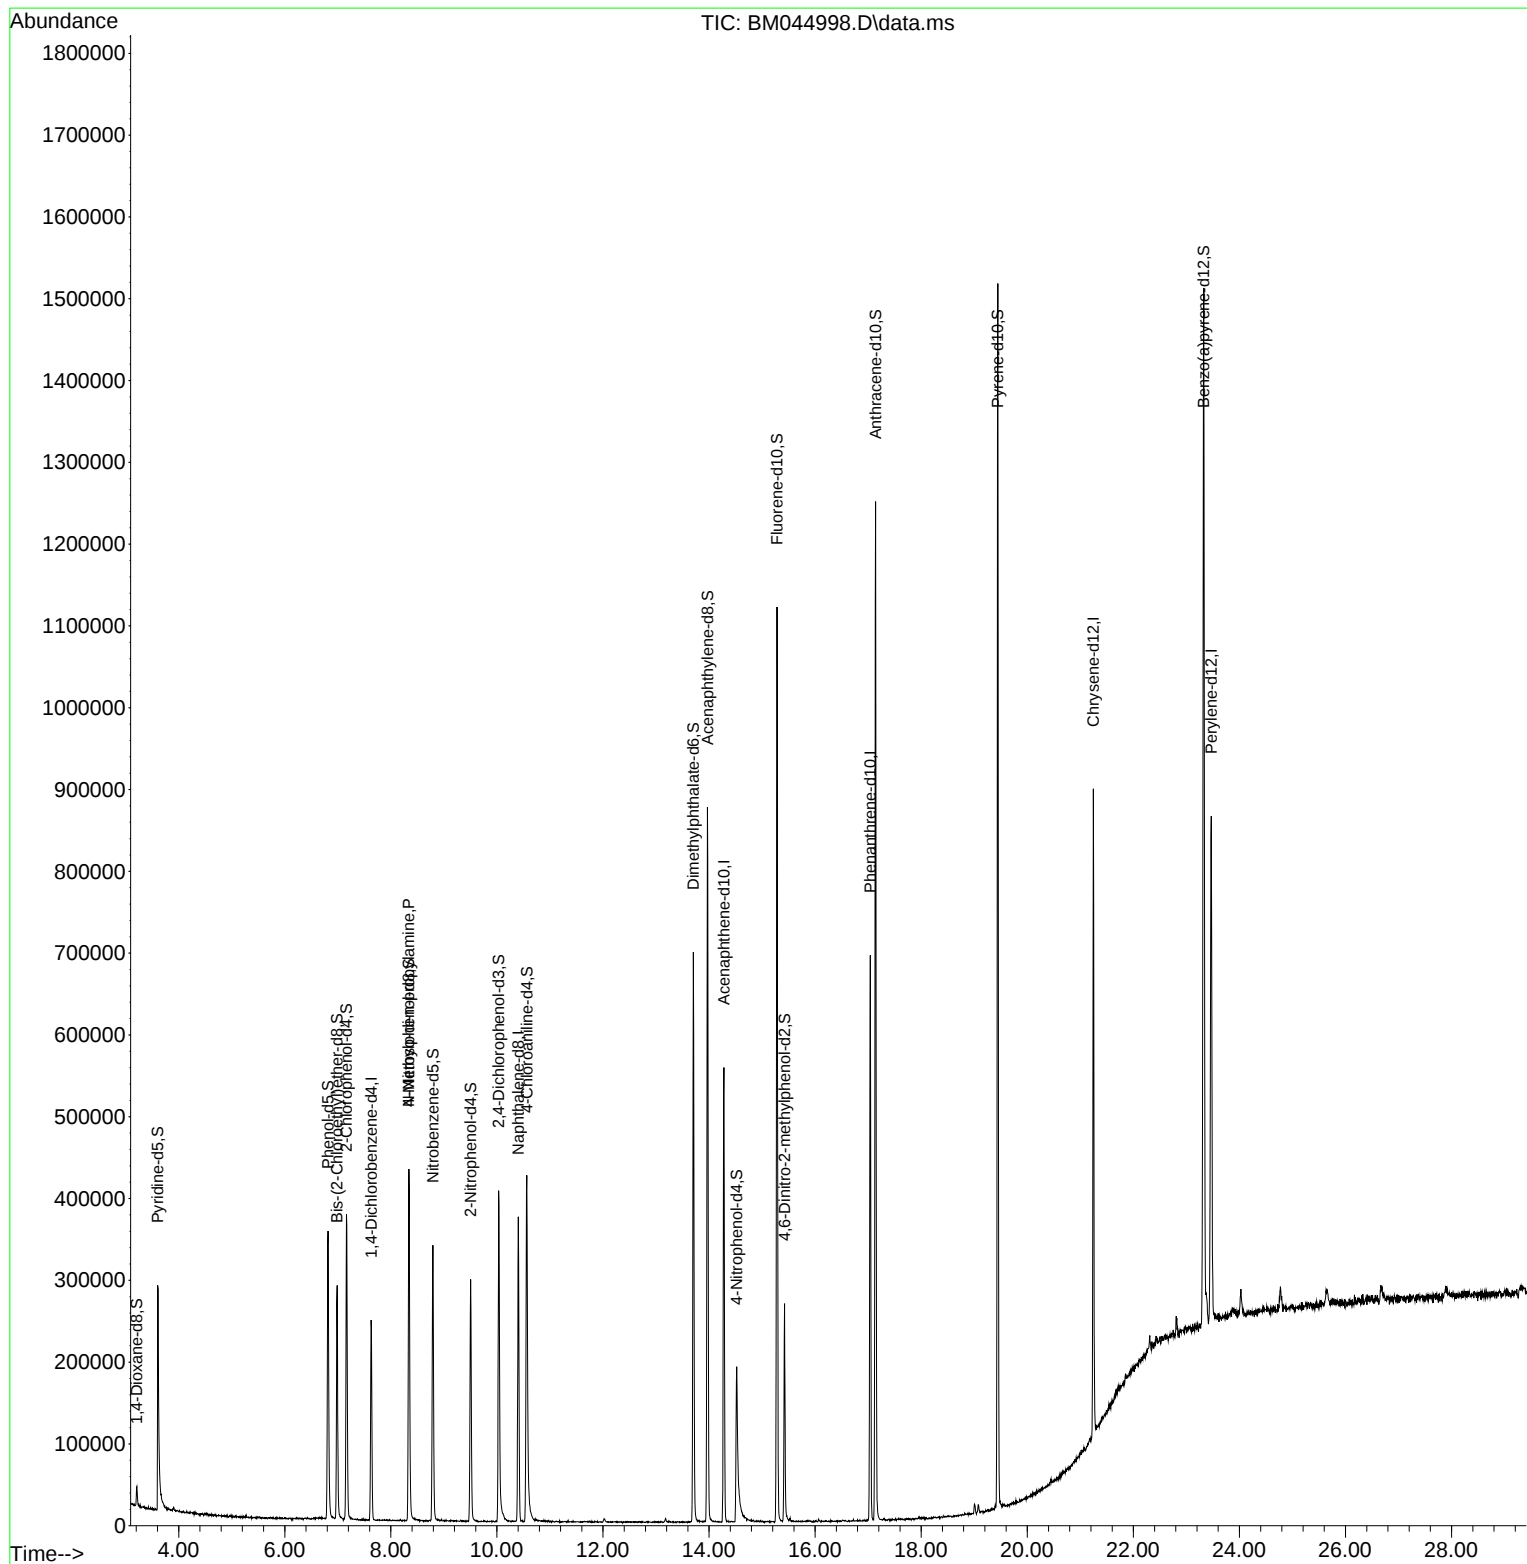

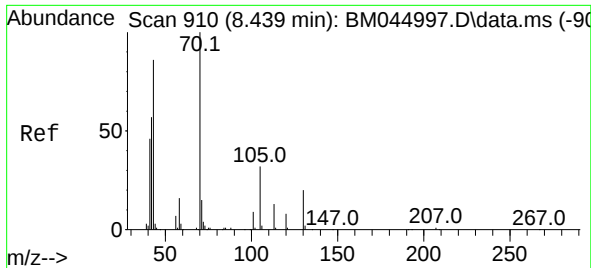

#17
N-Nitroso-di-n-propylamine
Concen: 1.427 ng/ul
RT: 8.339 min Scan# 80
Delta R.T. -0.100 min
Lab File: BM044998.D
Acq: 07 Apr 2024 08:48

Instrument :
BNA_M
ClientSampleId :

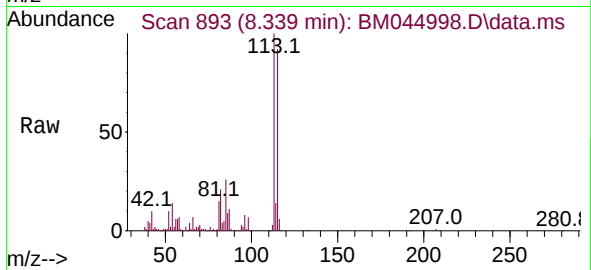

Tgt Ion: 70	Resp: 4753
Ion Ratio	Lower Upper
70	100
42	351.7 43.2 64.8#
101	0.0 6.4 9.6#
130	0.0 16.2 24.2#

