

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
 Data File : BM044964.D
 Acq On : 06 Apr 2024 11:17
 Operator : MA/JU
 Sample : PB160051BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK051

Quant Time: Apr 08 01:49:25 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Apr 08 01:45:36 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.634	152	86969	20.000	ng/u1	0.00
20) Naphthalene-d8	10.410	136	396294	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.280	164	257850	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.045	188	492575	20.000	ng/u1	0.00
79) Chrysene-d12	21.250	240	394375	20.000	ng/u1	0.00
88) Perylene-d12	23.474	264	460929	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.210	96	13385	5.747	ng/uL	0.00
4) Pyridine-d5	3.604	84	194475	30.706	ng/u1	0.00
7) Phenol-d5	6.816	99	231466	31.394	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	6.987	67	148845	33.885	ng/u1	0.00
11) 2-Chlorophenol-d4	7.169	132	196649	34.045	ng/u1	0.00
15) 4-Methylphenol-d8	8.339	113	192516	33.359	ng/u1	0.00
21) Nitrobenzene-d5	8.798	128	98519	32.365	ng/u1	0.00
24) 2-Nitrophenol-d4	9.510	143	111278	34.634	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.039	165	180159	30.583	ng/u1	0.00
31) 4-Chloroaniline-d4	10.563	131	322613	34.398	ng/u1	0.00
46) Dimethylphthalate-d6	13.710	166	611839	34.079	ng/u1	0.00
49) Acenaphthylene-d8	13.974	160	690811	32.571	ng/u1	0.00
54) 4-Nitrophenol-d4	14.516	143	80073	21.371	ng/u1	0.00
60) Fluorene-d10	15.286	176	501821	31.352	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.427	200	77575	26.561	ng/u1	0.00
73) Anthracene-d10	17.145	188	745907	33.662	ng/u1	0.00
81) Pyrene-d10	19.450	212	773973	39.857	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.333	264	772519	34.356	ng/u1	0.00


Target Compounds					Qvalue
17) N-Nitroso-di-n-propyla...	8.339	70	5057	1.142 ng/u1#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM044964.D
Acq On : 06 Apr 2024 11:17
Operator : MA/JU
Sample : PB160051BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK051

Quant Time: Apr 08 01:49:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Apr 08 01:45:36 2024
Response via : Initial Calibration

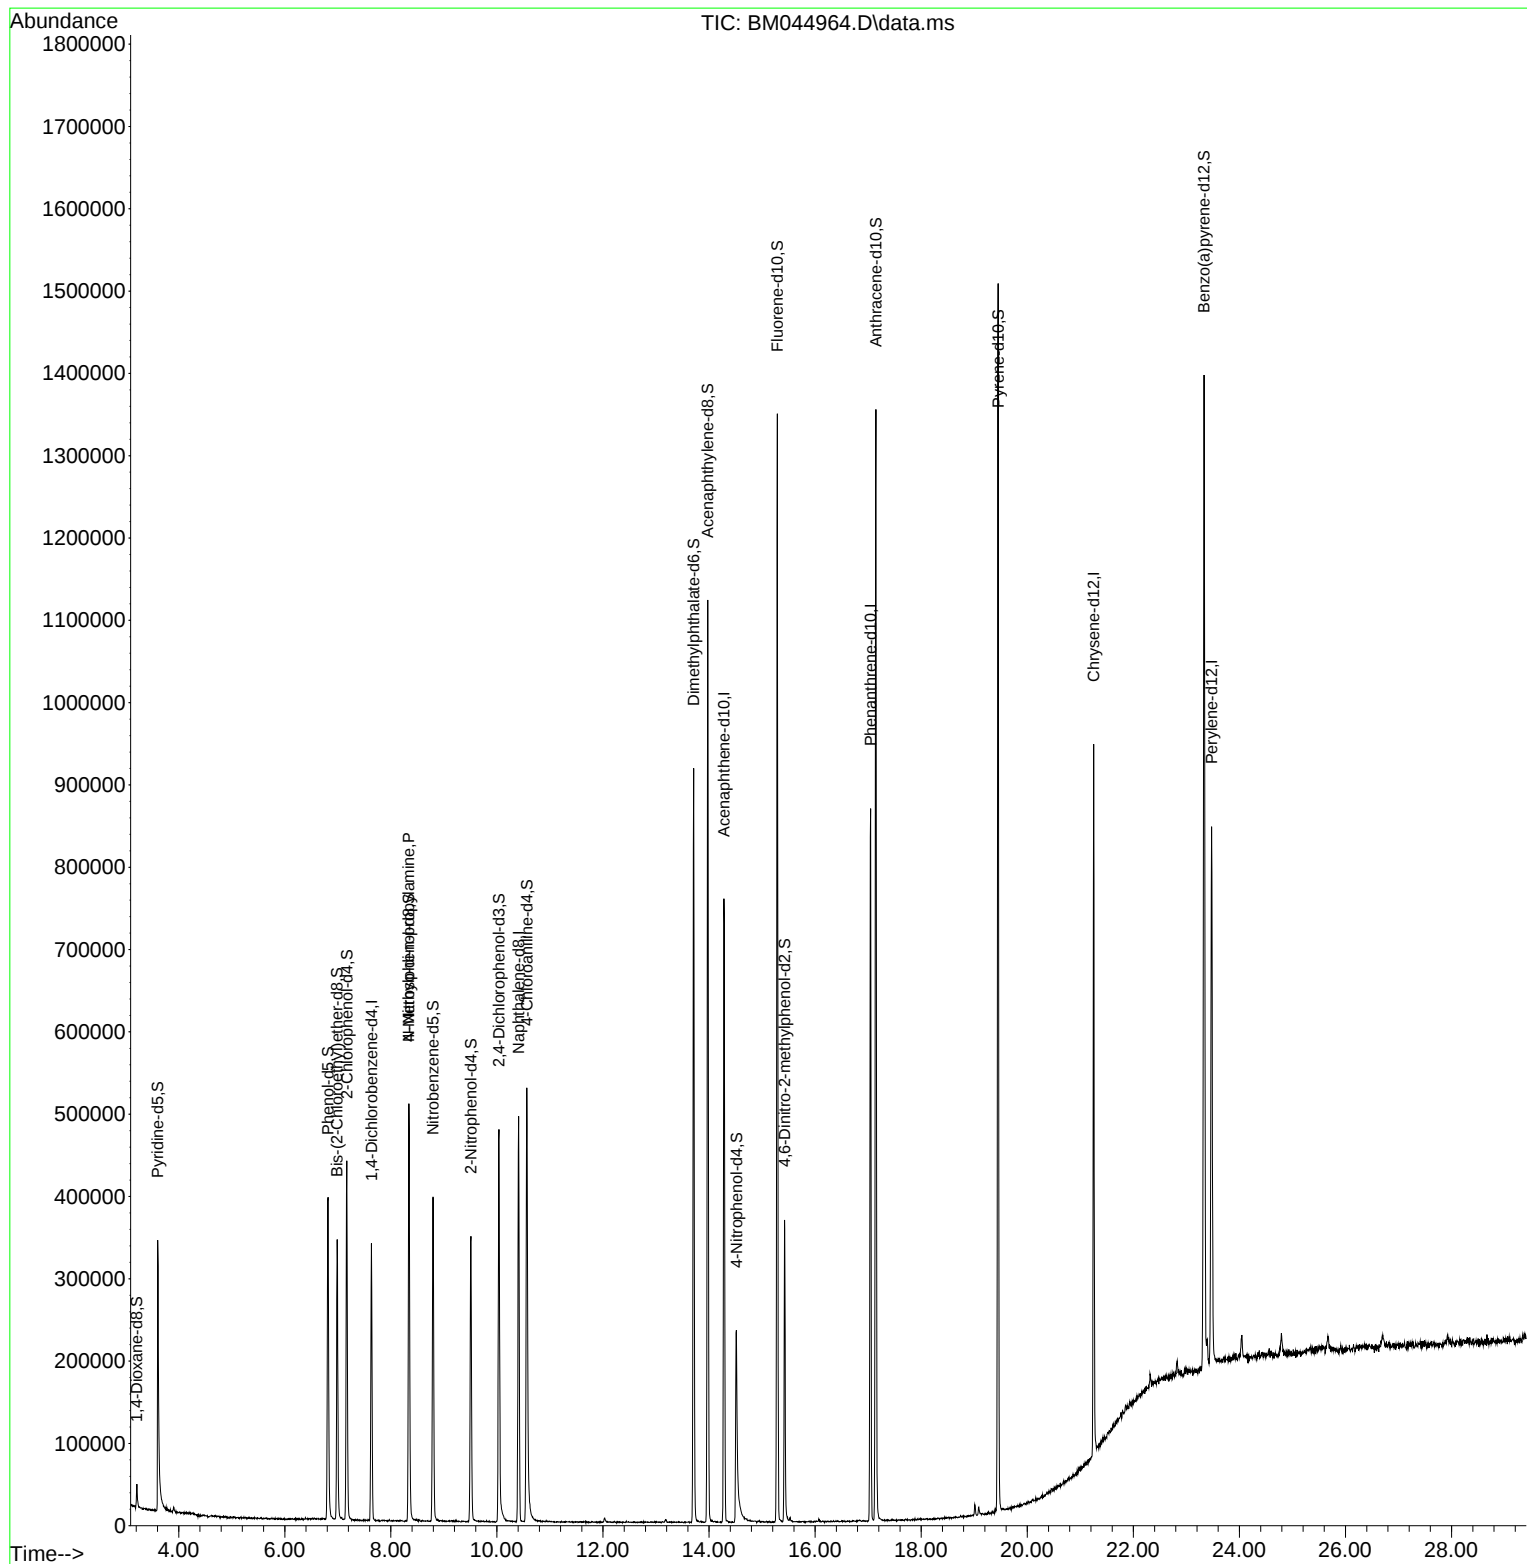

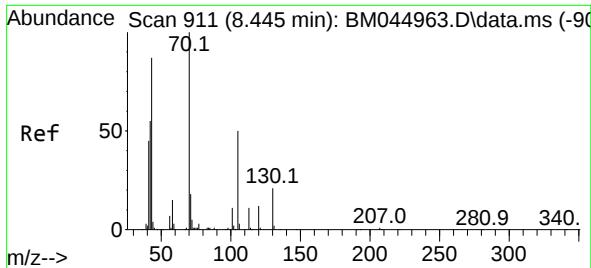

#17
N-Nitroso-di-n-propylamine
Concen: 1.142 ng/ul
RT: 8.339 min Scan# 893
Delta R.T. -0.106 min
Lab File: BM044964.D
Acq: 06 Apr 2024 11:17

Instrument :
BNA_M
ClientSampleId :
SBLK051

Tgt Ion: 70 Resp: 5057
Ion Ratio Lower Upper
70 100
42 371.3 43.2 64.8#
101 0.0 6.4 9.6#
130 0.0 16.2 24.2#

