

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
 Data File : BM044964.D
 Acq On : 06 Apr 2024 11:17
 Operator : MA/JU
 Sample : PB160051BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK051

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044964.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.210	17	21	29	rBV	29499	40560	1.92%	0.164%
2	3.604	85	88	106	rBV	328253	541378	25.66%	2.183%
3	3.904	137	139	145	rVB5	6597	8466	0.40%	0.034%
4	6.816	626	634	652	rBV	391405	679756	32.21%	2.741%
5	6.987	657	663	674	rBV	339474	542805	25.72%	2.189%
6	7.169	687	694	704	rBV	435434	688558	32.63%	2.777%
7	7.634	766	773	786	rBV	337191	532458	25.23%	2.147%
8	8.339	885	893	906	rBV	507390	851801	40.37%	3.435%
9	8.792	963	970	981	rBV	393845	676578	32.06%	2.728%
10	9.510	1084	1092	1103	rBV	346979	595746	28.23%	2.402%
11	10.039	1175	1182	1203	rBV	476061	867921	41.13%	3.500%
12	10.410	1238	1245	1257	rBV	492610	818397	38.78%	3.300%
13	10.563	1263	1271	1298	rBV	527153	1066940	50.56%	4.303%
14	11.663	1453	1458	1460	rVB4	2331	3251	0.15%	0.013%
15	11.792	1476	1480	1484	rBV5	1520	2679	0.13%	0.011%
16	12.033	1515	1521	1527	rBV5	5220	10373	0.49%	0.042%
17	12.380	1577	1580	1583	rBV2	1533	2219	0.11%	0.009%
18	13.116	1703	1705	1711	rBV4	1645	3037	0.14%	0.012%
19	13.186	1711	1717	1720	rVB5	3506	6626	0.31%	0.027%
20	13.710	1798	1806	1819	rVV	916529	1324300	62.76%	5.340%
21	13.974	1844	1851	1864	rBV	1119985	1612920	76.44%	6.504%
22	14.280	1897	1903	1912	rBV	757228	1132313	53.66%	4.566%
23	14.345	1912	1914	1919	rVB5	2235	3496	0.17%	0.014%
24	14.516	1934	1943	1966	rBV	233734	558776	26.48%	2.253%
25	15.133	2044	2048	2051	rBV5	1725	2139	0.10%	0.009%
26	15.286	2066	2074	2082	rBV	1346742	1921302	91.05%	7.748%
27	15.421	2091	2097	2109	rBV	366925	548871	26.01%	2.213%
28	15.527	2112	2115	2118	rVB4	4149	4704	0.22%	0.019%
29	16.068	2204	2207	2212	rVB5	3574	4122	0.20%	0.017%
30	16.198	2226	2229	2232	rBV4	1843	2914	0.14%	0.012%
31	17.045	2366	2373	2383	rBV	865535	1216441	57.65%	4.905%
32	17.145	2383	2390	2401	rBV	1349495	1954637	92.63%	7.882%
33	17.504	2448	2451	2456	rVB6	1394	2151	0.10%	0.009%
34	17.815	2500	2504	2506	rBV4	1525	2352	0.11%	0.009%
35	18.586	2633	2635	2639	rBV3	1505	2487	0.12%	0.010%
36	18.868	2680	2683	2685	rBV4	2317	2702	0.13%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM044964.D
Acq On : 06 Apr 2024 11:17
Operator : MA/JU
Sample : PB160051BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK051

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Title : SVOA CALIBRATION

37	19.009	2704	2707	2714	rVB4	13193	18030	0.85%	0.073%
38	19.086	2716	2720	2724	rBV3	9390	13325	0.63%	0.054%
39	19.339	2761	2763	2765	rBV3	3628	3345	0.16%	0.013%
40	19.398	2771	2773	2775	rBV2	3786	2590	0.12%	0.010%
41	19.450	2776	2782	2792	rVV	1490379	2029582	96.18%	8.184%
42	21.250	3083	3088	3097	rBV	864990	1146973	54.36%	4.625%
43	23.333	3435	3442	3450	rBV2	1204949	2110112	100.00%	8.509%
44	23.474	3460	3466	3478	rVB	647756	1237811	58.66%	4.992%




Sum of corrected areas: 24797944

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM044964.D
Acq On : 06 Apr 2024 11:17
Operator : MA/JU
Sample : PB160051BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK051

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

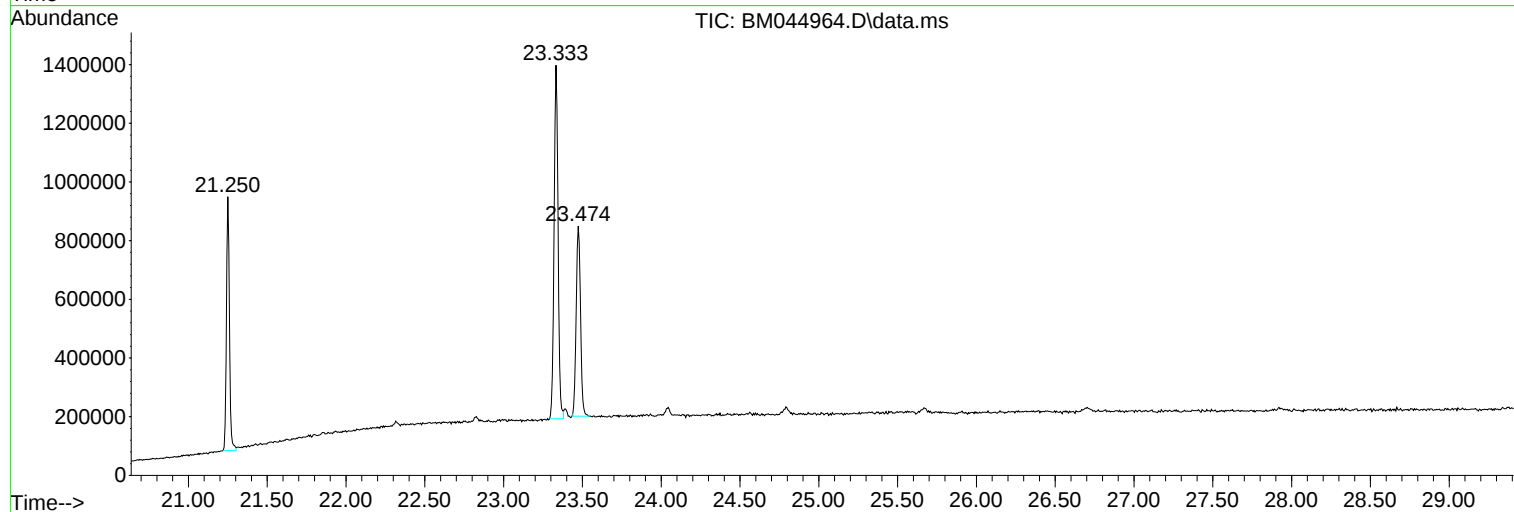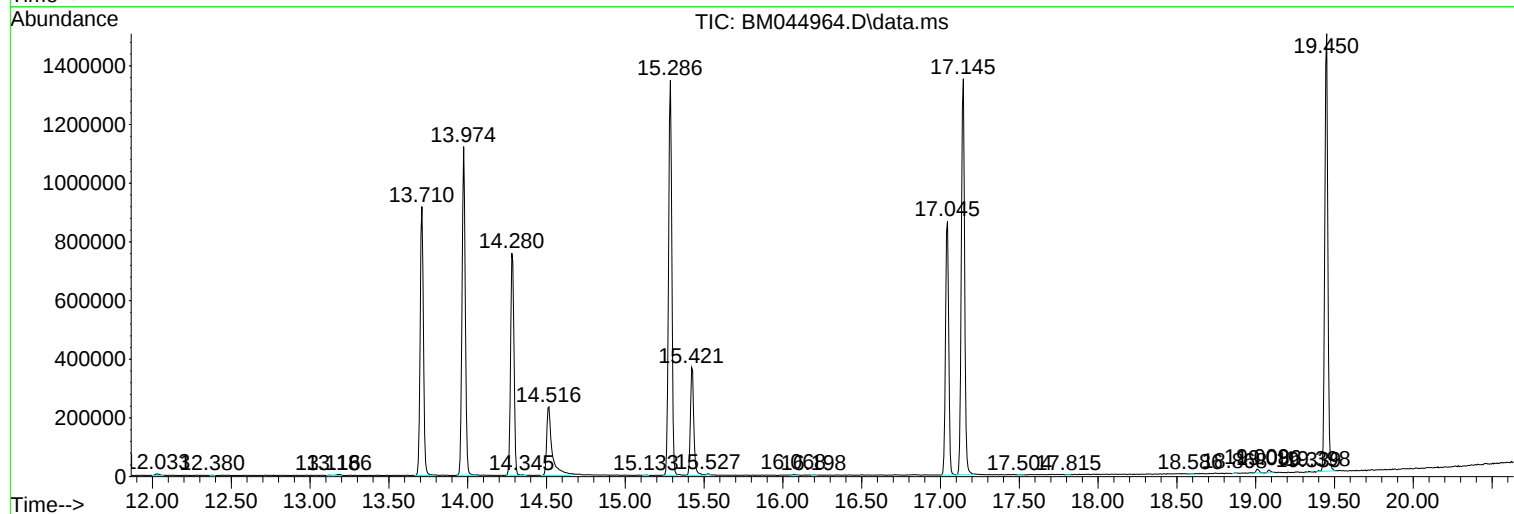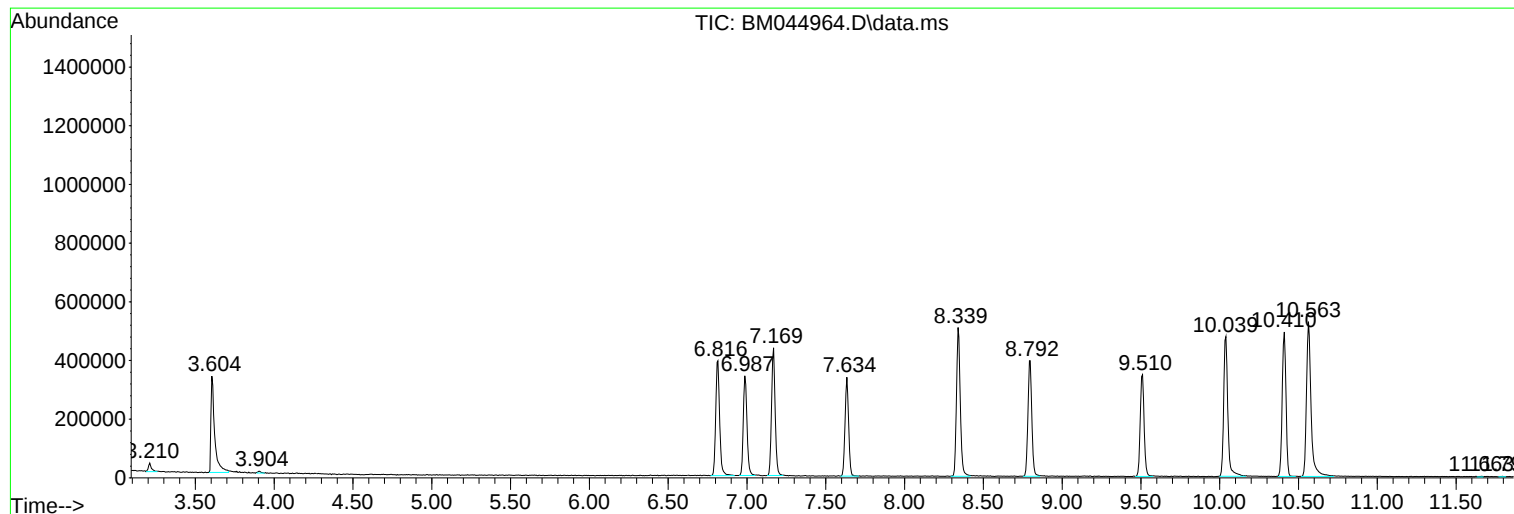

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM044964.D
Acq On : 06 Apr 2024 11:17
Operator : MA/JU
Sample : PB160051BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK051

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM044964.D
Acq On : 06 Apr 2024 11:17
Operator : MA/JU
Sample : PB160051BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK051

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc