

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
 Data File : BM044965.D
 Acq On : 06 Apr 2024 11:52
 Operator : MA/JU
 Sample : PB160048BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK048

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044965.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.210	18	21	27	rVB	16622	24729	1.73%	0.153%
2	3.610	86	89	102	rBV	189322	319054	22.34%	1.969%
3	3.899	136	138	143	rVB5	4617	7341	0.51%	0.045%
4	3.940	143	145	147	rBV3	2215	1927	0.13%	0.012%
5	4.034	159	161	163	rVB3	2868	1901	0.13%	0.012%
6	4.140	177	179	181	rVB3	2489	1881	0.13%	0.012%
7	4.557	248	250	253	rBV4	1485	1931	0.14%	0.012%
8	4.946	315	316	318	rBV2	1912	1572	0.11%	0.010%
9	5.269	367	371	372	rVB3	1588	1867	0.13%	0.012%
10	5.781	455	458	460	rBV4	1460	1533	0.11%	0.009%
11	6.257	538	539	542	rBV2	1694	1452	0.10%	0.009%
12	6.522	581	584	585	rBV3	1804	1667	0.12%	0.010%
13	6.816	626	634	647	rBV	230694	409524	28.67%	2.527%
14	6.987	657	663	673	rBV	193971	320497	22.44%	1.978%
15	7.169	687	694	707	rVB	259492	422233	29.56%	2.606%
16	7.316	717	719	722	rBV3	1597	1734	0.12%	0.011%
17	7.634	766	773	782	rBV	277013	443771	31.07%	2.739%
18	8.345	887	894	904	rBV	279035	489660	34.28%	3.022%
19	8.545	927	928	931	rVB2	2423	1747	0.12%	0.011%
20	8.798	964	971	981	rVV	220737	389057	27.24%	2.401%
21	8.863	981	982	988	rVB4	2499	2279	0.16%	0.014%
22	9.157	1030	1032	1036	rVB4	1939	2165	0.15%	0.013%
23	9.281	1049	1053	1055	rBV4	1874	2238	0.16%	0.014%
24	9.392	1069	1072	1076	rVB4	1133	1615	0.11%	0.010%
25	9.451	1080	1082	1085	rVB3	1733	1727	0.12%	0.011%
26	9.510	1085	1092	1101	rBV	191574	329513	23.07%	2.033%
27	9.675	1119	1120	1125	rVB5	1300	1587	0.11%	0.010%
28	9.734	1127	1130	1135	rVB5	1126	1483	0.10%	0.009%
29	10.039	1174	1182	1196	rBV	258781	484493	33.92%	2.990%
30	10.169	1203	1204	1207	rVB3	2541	1510	0.11%	0.009%
31	10.328	1228	1231	1233	rBV4	1486	1723	0.12%	0.011%
32	10.410	1238	1245	1252	rVV	385762	638782	44.72%	3.942%
33	10.569	1264	1272	1286	rBV	221100	490915	34.37%	3.029%
34	10.792	1308	1310	1314	rBV4	1904	2042	0.14%	0.013%
35	10.881	1323	1325	1329	rVB5	1497	1933	0.14%	0.012%
36	10.922	1329	1332	1335	rBV4	1201	1496	0.10%	0.009%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
 Data File : BM044965.D
 Acq On : 06 Apr 2024 11:52
 Operator : MA/JU
 Sample : PB160048BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK048

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	11.192	1375	1378	1380	rBV4	1118	1433	0.10%	0.009%
38	11.439	1417	1420	1424	rVB4	1696	2127	0.15%	0.013%
39	11.504	1429	1431	1436	rBV5	1628	2781	0.19%	0.017%
40	12.028	1517	1520	1522	rVV4	1990	3082	0.22%	0.019%
41	12.045	1522	1523	1526	rVB3	2301	1829	0.13%	0.011%
42	12.469	1594	1595	1599	rVB3	1653	1475	0.10%	0.009%
43	13.180	1714	1716	1720	rVV4	2293	2895	0.20%	0.018%
44	13.710	1800	1806	1823	rVB	469747	693543	48.56%	4.280%
45	13.974	1843	1851	1863	rBV	609430	897765	62.86%	5.540%
46	14.222	1889	1893	1897	rBV4	1300	1599	0.11%	0.010%
47	14.280	1897	1903	1911	rBV	572839	850614	59.56%	5.249%
48	14.521	1937	1944	1961	rBV3	101412	281077	19.68%	1.735%
49	14.833	1995	1997	2000	rVB3	2034	1585	0.11%	0.010%
50	14.886	2002	2006	2009	rBV4	1539	2660	0.19%	0.016%
51	14.986	2018	2023	2025	rBV3	1029	1740	0.12%	0.011%
52	15.086	2035	2040	2043	rVB3	1685	2327	0.16%	0.014%
53	15.286	2067	2074	2086	rVV	758844	1095961	76.73%	6.763%
54	15.421	2091	2097	2109	rVV	176187	278016	19.47%	1.716%
55	15.516	2111	2113	2114	rVV2	2837	2504	0.18%	0.015%
56	15.533	2114	2116	2120	rVV4	3237	3490	0.24%	0.022%
57	15.574	2120	2123	2125	rVV3	1547	1838	0.13%	0.011%
58	15.857	2167	2171	2173	rBV4	1183	1750	0.12%	0.011%
59	16.074	2206	2208	2211	rBV3	1846	1672	0.12%	0.010%
60	16.345	2251	2254	2257	rBV4	1414	1537	0.11%	0.009%
61	16.580	2292	2294	2296	rBV2	1672	1766	0.12%	0.011%
62	16.715	2316	2317	2321	rVB4	2063	2165	0.15%	0.013%
63	16.757	2321	2324	2325	rBV3	1551	1543	0.11%	0.010%
64	16.821	2333	2335	2339	rBV4	2375	2810	0.20%	0.017%
65	17.039	2366	2372	2383	rBV	667592	984112	68.90%	6.073%
66	17.145	2383	2390	2401	rBV	800788	1176909	82.40%	7.263%
67	17.727	2487	2489	2492	rBV3	2242	2721	0.19%	0.017%
68	17.827	2503	2506	2508	rBV4	1460	1752	0.12%	0.011%
69	17.921	2521	2522	2525	rBV4	1435	1565	0.11%	0.010%
70	18.462	2612	2614	2616	rBV2	1477	1569	0.11%	0.010%
71	18.492	2617	2619	2623	rVB5	2421	2626	0.18%	0.016%
72	18.533	2623	2626	2628	rBV4	2456	2936	0.21%	0.018%
73	18.798	2670	2671	2673	rBV2	2011	1839	0.13%	0.011%
74	19.015	2703	2708	2712	rBV6	9151	11309	0.79%	0.070%
75	19.086	2716	2720	2724	rBV2	6289	8202	0.57%	0.051%
76	19.198	2736	2739	2740	rBV3	2088	2804	0.20%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM044965.D
Acq On : 06 Apr 2024 11:52
Operator : MA/JU
Sample : PB160048BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK048

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M

Title : SVOA CALIBRATION

77	19.398	2771	2773	2776	rBV4	2764	2762	0.19%	0.017%
78	19.451	2776	2782	2792	rVV	927595	1325916	92.84%	8.182%
79	21.250	3083	3088	3098	rBV	804184	1073638	75.17%	6.625%
80	23.333	3436	3442	3449	rBV2	799821	1428244	100.00%	8.814%
81	23.474	3460	3466	3477	rVB	639553	1221713	85.54%	7.539%


Sum of corrected areas: 16204780

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM044965.D
Acq On : 06 Apr 2024 11:52
Operator : MA/JU
Sample : PB160048BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK048

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

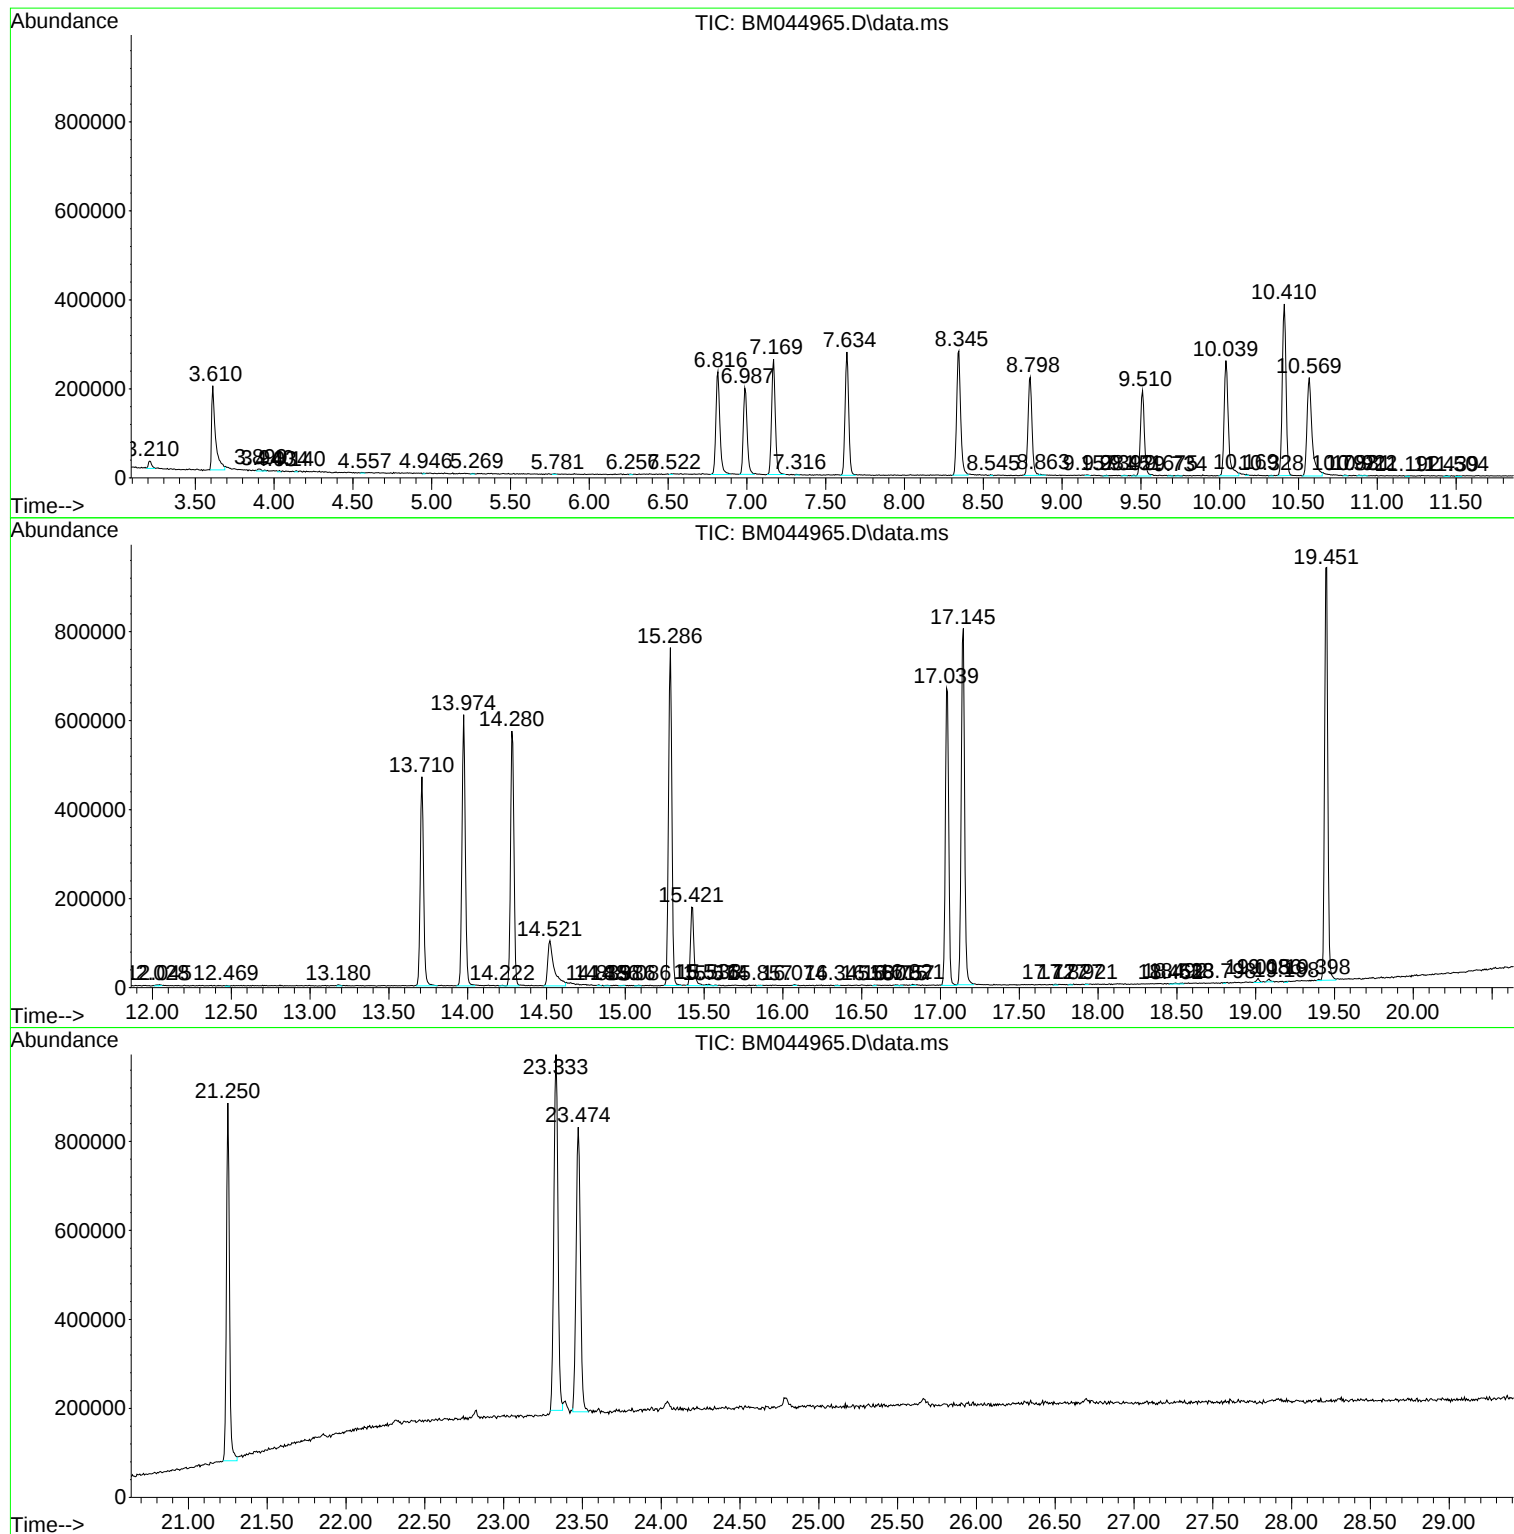

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM044965.D
Acq On : 06 Apr 2024 11:52
Operator : MA/JU
Sample : PB160048BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK048

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM044965.D
Acq On : 06 Apr 2024 11:52
Operator : MA/JU
Sample : PB160048BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK048

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc