

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
 Data File : BM044981.D
 Acq On : 06 Apr 2024 22:03
 Operator : MA/JU
 Sample : PB160053BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK053

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044981.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.210	17	21	28	rVB	25891	38748	1.50%	0.157%
2	3.605	85	88	106	rBV	287376	506191	19.64%	2.050%
3	3.905	137	139	143	rVB2	6100	6484	0.25%	0.026%
4	5.757	452	454	458	rBV4	1937	3109	0.12%	0.013%
5	6.099	508	512	514	rBV5	1798	2599	0.10%	0.011%
6	6.257	535	539	542	rBV5	1952	2723	0.11%	0.011%
7	6.816	627	634	646	rBV	370002	629416	24.43%	2.549%
8	6.987	657	663	675	rBV	294827	475258	18.44%	1.924%
9	7.169	685	694	703	rBV	384483	632771	24.56%	2.562%
10	7.634	767	773	781	rBV	304685	475842	18.47%	1.927%
11	8.345	887	894	909	rVV	451036	778006	30.19%	3.150%
12	8.628	939	942	945	rVB4	2542	2957	0.11%	0.012%
13	8.651	945	946	950	rBV3	2221	3101	0.12%	0.013%
14	8.792	963	970	980	rBV	350681	605454	23.50%	2.452%
15	9.328	1059	1061	1066	rVB4	1663	2705	0.10%	0.011%
16	9.504	1084	1091	1101	rBV	305871	535580	20.79%	2.169%
17	9.622	1109	1111	1116	rVB3	2146	2681	0.10%	0.011%
18	10.039	1174	1182	1199	rBV	436363	800864	31.08%	3.243%
19	10.410	1237	1245	1256	rVB	426465	729607	28.32%	2.954%
20	10.563	1264	1271	1294	rBV	467307	952305	36.96%	3.856%
21	11.298	1392	1396	1401	rVB6	1827	3989	0.15%	0.016%
22	12.028	1514	1520	1524	rBV7	4101	9150	0.36%	0.037%
23	13.180	1712	1716	1720	rBV4	4383	6189	0.24%	0.025%
24	13.710	1798	1806	1818	rBV	754080	1109870	43.07%	4.494%
25	13.822	1823	1825	1830	rVB5	1713	2804	0.11%	0.011%
26	13.974	1844	1851	1864	rVB	977213	1432009	55.58%	5.798%
27	14.110	1870	1874	1878	rVB6	1782	3140	0.12%	0.013%
28	14.280	1896	1903	1913	rBV	674079	1000384	38.82%	4.051%
29	14.521	1937	1944	1969	rBV	243852	609067	23.64%	2.466%
30	15.286	2066	2074	2087	rVV	1223399	1767682	68.60%	7.158%
31	15.421	2087	2097	2113	rVV	370096	560515	21.75%	2.270%
32	15.527	2113	2115	2121	rVB5	5642	7532	0.29%	0.030%
33	16.833	2333	2337	2341	rBV5	2696	4146	0.16%	0.017%
34	17.039	2366	2372	2379	rBV	846877	1214411	47.13%	4.917%
35	17.139	2383	2389	2401	rBV2	1345413	1966382	76.31%	7.962%
36	17.339	2419	2423	2426	rBV6	1952	3070	0.12%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM044981.D
Acq On : 06 Apr 2024 22:03
Operator : MA/JU
Sample : PB160053BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK053

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Title : SVOA CALIBRATION

37	17.445	2437	2441	2443	rBV4	1849	2959	0.11%	0.012%
38	17.962	2526	2529	2534	rBV6	3108	4479	0.17%	0.018%
39	18.286	2582	2584	2587	rBV3	2319	2853	0.11%	0.012%
40	18.480	2615	2617	2620	rBV3	3048	3947	0.15%	0.016%
41	18.651	2643	2646	2649	rBV5	2067	2712	0.11%	0.011%
42	18.892	2685	2687	2689	rBV3	2428	2614	0.10%	0.011%
43	19.009	2703	2707	2712	rBV3	15685	22250	0.86%	0.090%
44	19.080	2715	2719	2724	rBV	13176	18917	0.73%	0.077%
45	19.245	2745	2747	2750	rBV4	3702	4700	0.18%	0.019%
46	19.398	2770	2773	2775	rBV4	5330	6432	0.25%	0.026%
47	19.445	2775	2781	2791	rVV	1675778	2292997	88.99%	9.285%
48	21.250	3083	3088	3095	rBV	1013256	1339654	51.99%	5.424%
49	23.333	3435	3442	3448	rBV2	1425742	2576707	100.00%	10.434%
50	23.468	3460	3465	3475	rVB	786158	1528509	59.32%	6.189%




Sum of corrected areas: 24696471

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM044981.D
Acq On : 06 Apr 2024 22:03
Operator : MA/JU
Sample : PB160053BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK053

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

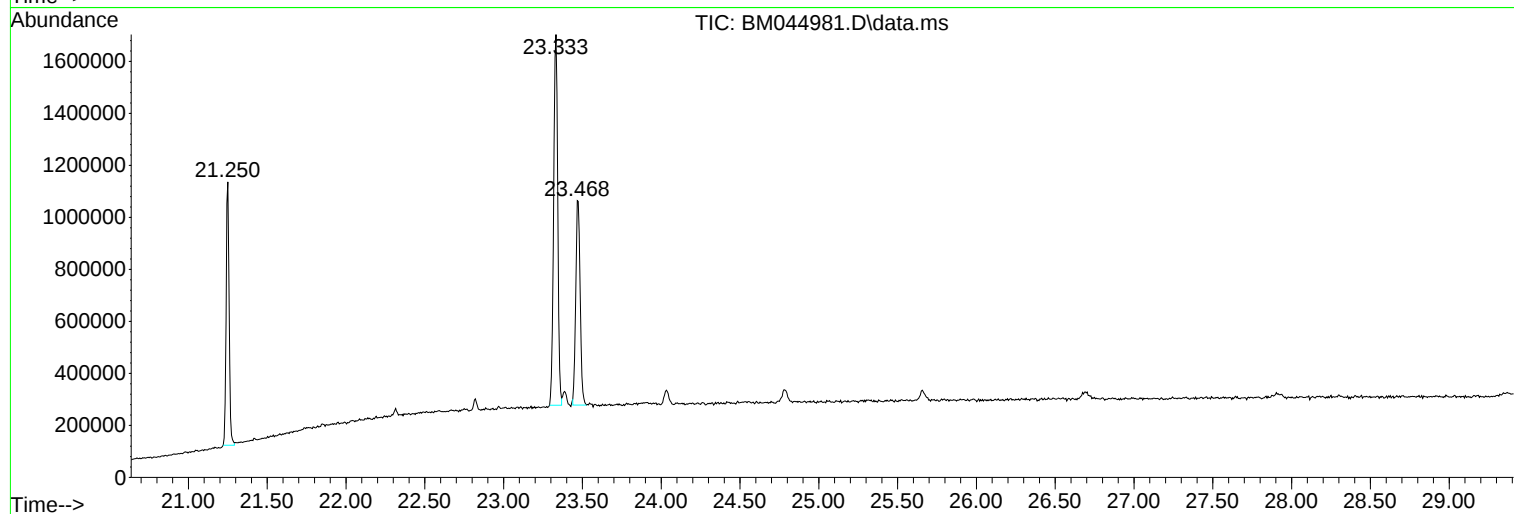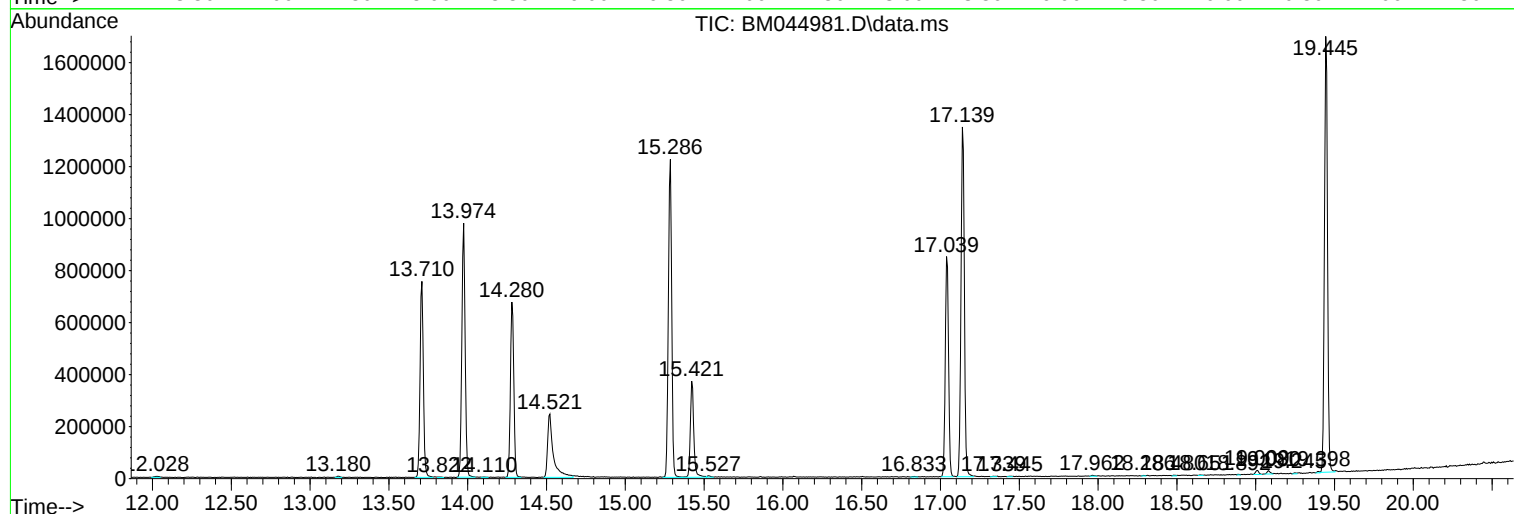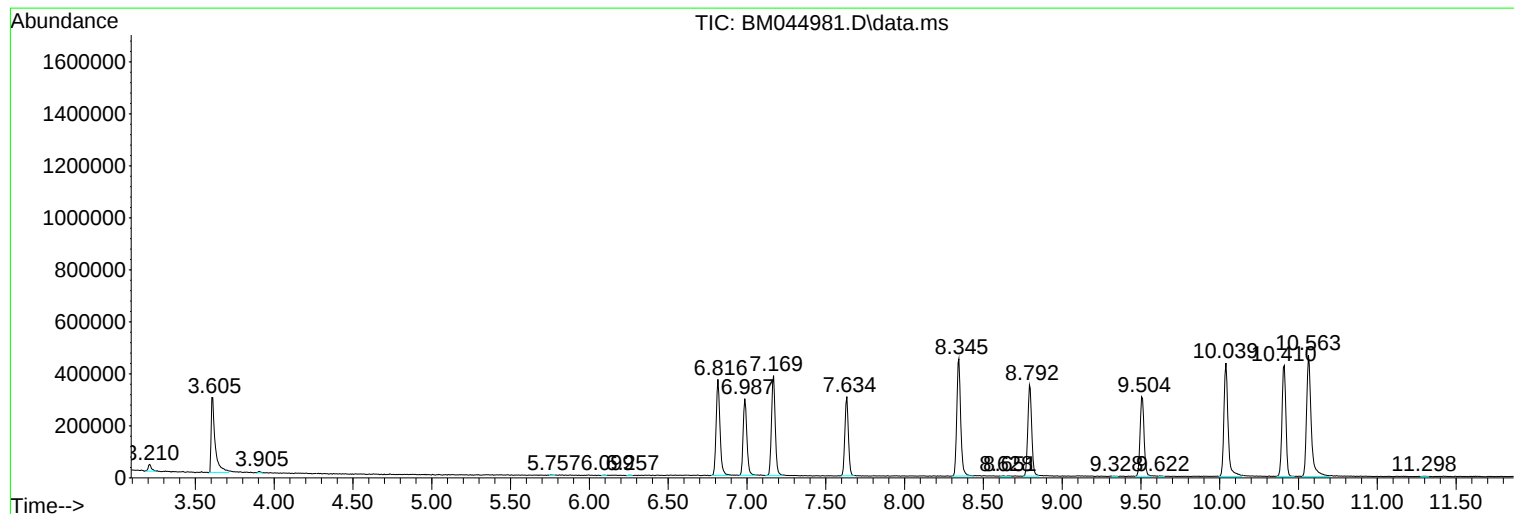

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM044981.D
Acq On : 06 Apr 2024 22:03
Operator : MA/JU
Sample : PB160053BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK053

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM044981.D
Acq On : 06 Apr 2024 22:03
Operator : MA/JU
Sample : PB160053BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK053

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------