

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
 Data File : BM044983.D
 Acq On : 06 Apr 2024 23:15
 Operator : MA/JU
 Sample : P2012-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AM5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044983.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.210	18	21	24	rBV	16320	19678	0.55%	0.075%
2	3.246	24	27	33	rVB2	14361	23040	0.64%	0.088%
3	3.622	88	91	100	rBV	56767	109493	3.06%	0.418%
4	3.898	136	138	143	rVB4	4690	4965	0.14%	0.019%
5	5.716	444	447	451	rVB4	4882	5495	0.15%	0.021%
6	6.816	629	634	644	rBV	67914	130767	3.65%	0.499%
7	6.987	657	663	671	rBV	327794	516165	14.42%	1.970%
8	7.169	687	694	705	rBV	315049	521061	14.56%	1.988%
9	7.634	767	773	780	rBV	277568	447646	12.51%	1.708%
10	8.345	888	894	907	rBV2	225143	394333	11.02%	1.505%
11	8.739	955	961	964	rBV3	7668	12227	0.34%	0.047%
12	8.792	964	970	981	rVV	382031	653680	18.27%	2.495%
13	8.951	995	997	1003	rVB7	2255	3675	0.10%	0.014%
14	9.504	1084	1091	1102	rBV	325492	574039	16.04%	2.191%
15	10.039	1174	1182	1194	rBV	431834	797358	22.28%	3.043%
16	10.357	1233	1236	1238	rBV3	3268	4906	0.14%	0.019%
17	10.410	1238	1245	1252	rVV	410662	689752	19.28%	2.632%
18	10.457	1252	1253	1259	rVB3	6499	6591	0.18%	0.025%
19	10.563	1264	1271	1286	rBV	353970	722745	20.20%	2.758%
20	11.092	1357	1361	1362	rBV3	3809	3650	0.10%	0.014%
21	11.239	1382	1386	1388	rBV4	3394	4191	0.12%	0.016%
22	11.292	1392	1395	1396	rBV3	3982	3672	0.10%	0.014%
23	11.669	1452	1459	1467	rVB5	6497	11697	0.33%	0.045%
24	11.963	1502	1509	1513	rBV3	10922	23620	0.66%	0.090%
25	12.010	1515	1517	1523	rVB4	6604	9712	0.27%	0.037%
26	12.269	1556	1561	1568	rBV6	5377	9814	0.27%	0.037%
27	12.363	1574	1577	1583	rVB6	2822	4988	0.14%	0.019%
28	12.892	1661	1667	1672	rVB8	2621	5173	0.14%	0.020%
29	13.098	1698	1702	1705	rBV5	3764	5045	0.14%	0.019%
30	13.180	1705	1716	1719	rVV5	5751	12604	0.35%	0.048%
31	13.245	1722	1727	1732	rVB8	2363	3897	0.11%	0.015%
32	13.516	1769	1773	1778	rBV5	2521	5411	0.15%	0.021%
33	13.710	1798	1806	1817	rBV	920885	1347370	37.65%	5.142%
34	13.974	1843	1851	1861	rBV	1150277	1660854	46.41%	6.338%
35	14.086	1866	1870	1872	rVV4	3441	4807	0.13%	0.018%
36	14.280	1896	1903	1913	rBV	635578	937891	26.21%	3.579%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
 Data File : BM044983.D
 Acq On : 06 Apr 2024 23:15
 Operator : MA/JU
 Sample : P2012-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AM5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	14.539	1942	1947	1956	rBV3	34004	89968	2.51%	0.343%
38	14.662	1966	1968	1972	rVB5	3127	3727	0.10%	0.014%
39	14.727	1976	1979	1983	rVB4	3526	4327	0.12%	0.017%
40	15.280	2067	2073	2081	rBV	1478528	2183676	61.02%	8.333%
41	15.421	2091	2097	2109	rBV	467335	699906	19.56%	2.671%
42	15.521	2111	2114	2119	rVB7	7559	10989	0.31%	0.042%
43	15.833	2164	2167	2172	rBV7	2298	4388	0.12%	0.017%
44	16.074	2204	2208	2211	rVB5	4735	6739	0.19%	0.026%
45	16.804	2328	2332	2334	rBV5	3021	3858	0.11%	0.015%
46	16.909	2349	2350	2356	rBV5	2852	4992	0.14%	0.019%
47	16.974	2356	2361	2365	rVV8	3962	7103	0.20%	0.027%
48	17.039	2366	2372	2379	rVV	806798	1122339	31.36%	4.283%
49	17.139	2383	2389	2402	rVV	1803970	2536306	70.88%	9.679%
50	17.345	2420	2424	2428	rVV7	2724	3594	0.10%	0.014%
51	17.445	2437	2441	2443	rBV5	2992	3868	0.11%	0.015%
52	17.821	2503	2505	2507	rBV3	3182	3784	0.11%	0.014%
53	17.915	2515	2521	2522	rBV5	5507	8023	0.22%	0.031%
54	17.951	2523	2527	2536	rVV2	42345	68511	1.91%	0.261%
55	18.198	2566	2569	2572	rBV4	2993	4060	0.11%	0.015%
56	19.009	2703	2707	2711	rVB3	24225	32375	0.90%	0.124%
57	19.086	2716	2720	2724	rVV2	17952	26761	0.75%	0.102%
58	19.245	2743	2747	2749	rBV3	19272	23257	0.65%	0.089%
59	19.445	2775	2781	2788	rBV	2328345	3116964	87.11%	11.895%
60	20.974	3039	3041	3046	rVB5	36704	39958	1.12%	0.152%
61	21.250	3083	3088	3096	rBV	998951	1358962	37.98%	5.186%
62	23.333	3435	3442	3449	rBV2	1972811	3578383	100.00%	13.656%
63	23.474	3459	3466	3477	rVB	801005	1565062	43.74%	5.973%




Sum of corrected areas: 26203892

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM044983.D
Acq On : 06 Apr 2024 23:15
Operator : MA/JU
Sample : P2012-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COAM5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

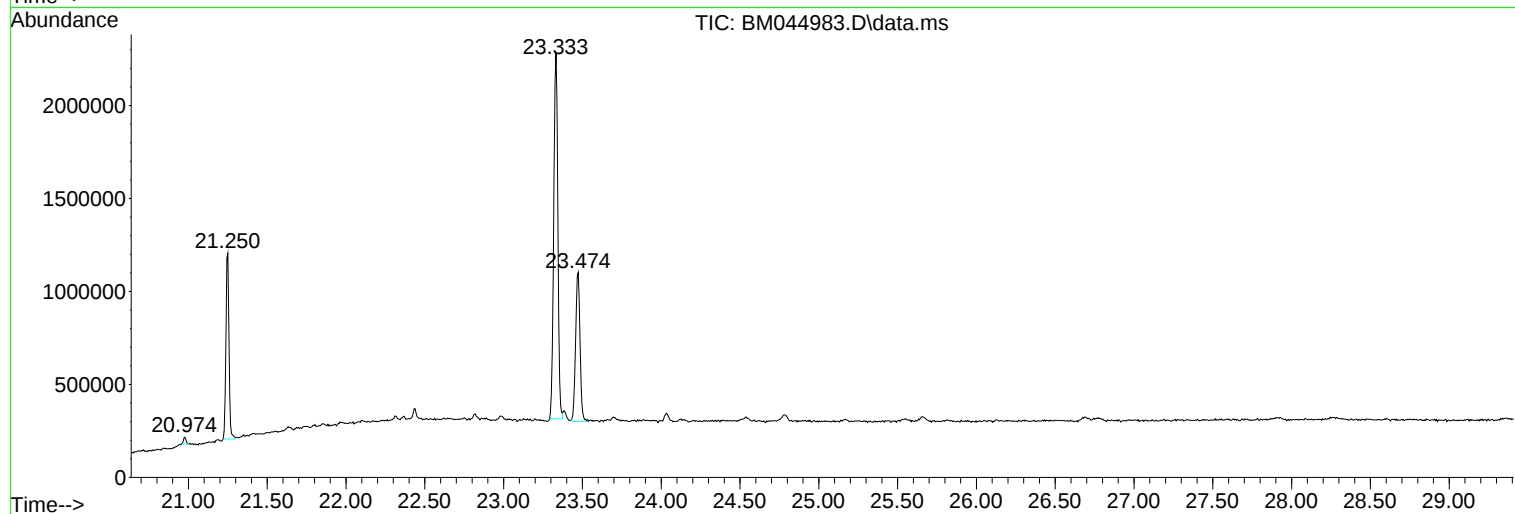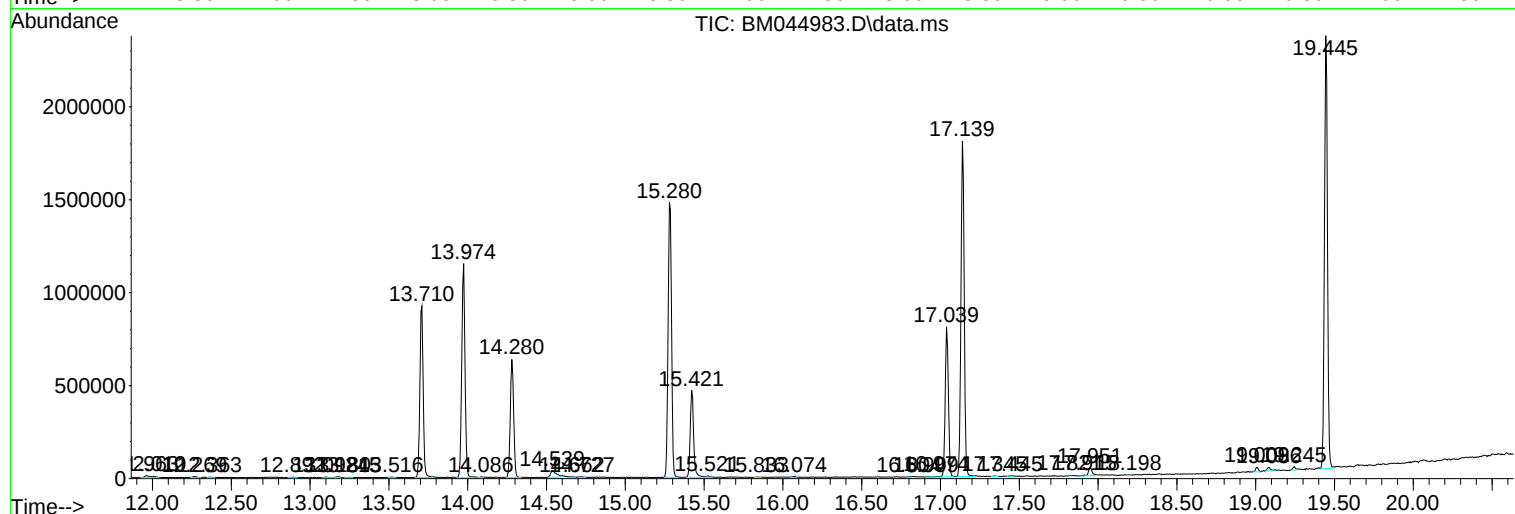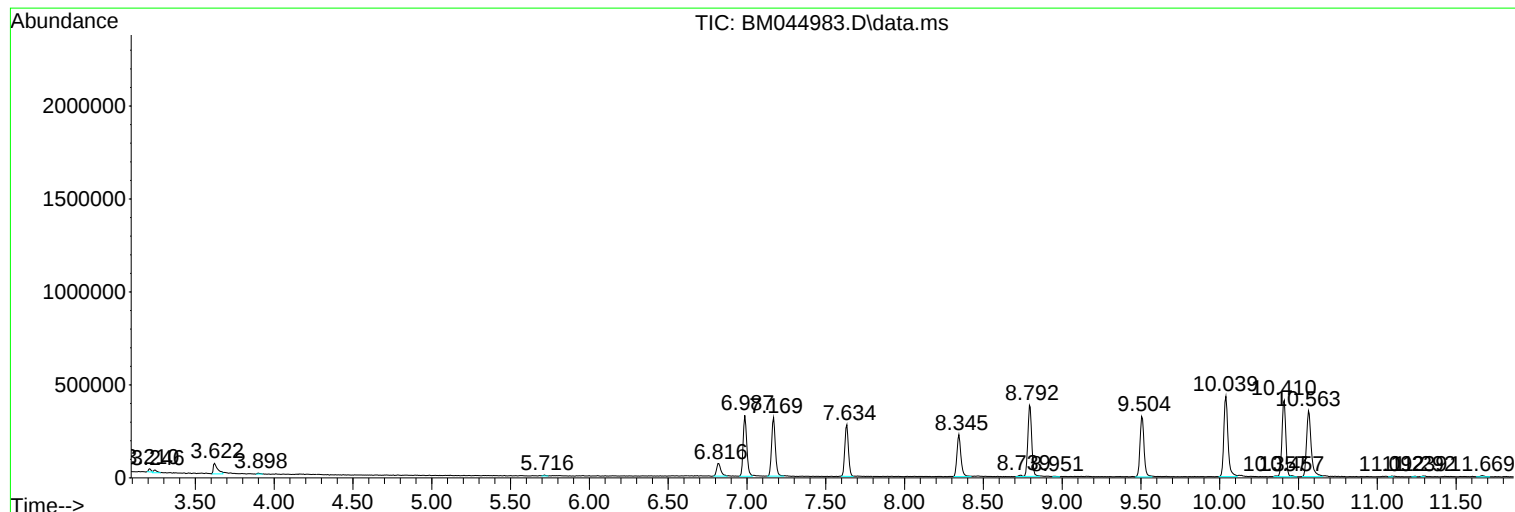

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM044983.D
Acq On : 06 Apr 2024 23:15
Operator : MA/JU
Sample : P2012-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AM5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM044983.D
Acq On : 06 Apr 2024 23:15
Operator : MA/JU
Sample : P2012-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AM5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc