

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
 Data File : BM044985.D
 Acq On : 07 Apr 2024 00:27
 Operator : MA/JU
 Sample : P2013-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EOM88

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044985.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	11	14	18	rBV	24321	29792	0.98%	0.118%
2	3.210	18	21	28	rVB	20447	29110	0.96%	0.115%
3	3.616	87	90	105	rBV	85110	158911	5.23%	0.629%
4	3.904	136	139	145	rVB4	7368	12674	0.42%	0.050%
5	4.281	199	203	204	rVB4	3481	4179	0.14%	0.017%
6	4.293	204	205	210	rVB4	2907	3785	0.12%	0.015%
7	4.404	219	224	232	rVB	87427	126607	4.17%	0.501%
8	4.710	274	276	281	rBV5	2383	3656	0.12%	0.014%
9	4.987	322	323	329	rVB5	3666	4976	0.16%	0.020%
10	5.175	351	355	360	rBV4	5051	6515	0.21%	0.026%
11	5.304	373	377	384	rBV2	9180	18813	0.62%	0.075%
12	5.663	434	438	443	rBV5	6657	9596	0.32%	0.038%
13	6.016	497	498	503	rBV4	2093	3180	0.10%	0.013%
14	6.816	628	634	645	rBV	83592	158280	5.21%	0.627%
15	6.987	657	663	678	rBV	367840	586724	19.31%	2.324%
16	7.169	687	694	704	rBV	354833	583272	19.20%	2.310%
17	7.234	704	705	710	rVB5	3349	3332	0.11%	0.013%
18	7.634	766	773	783	rBV	300972	493466	16.24%	1.954%
19	7.981	824	832	838	rVB8	4943	11079	0.36%	0.044%
20	8.345	886	894	908	rBV	252177	448253	14.75%	1.775%
21	8.792	962	970	977	rBV	421809	714180	23.51%	2.829%
22	9.504	1085	1091	1103	rBV	352055	597482	19.67%	2.366%
23	10.039	1175	1182	1200	rBV	438098	827712	27.25%	3.278%
24	10.269	1217	1221	1228	rVB7	5648	10349	0.34%	0.041%
25	10.404	1237	1244	1252	rBV	423775	718760	23.66%	2.847%
26	10.563	1264	1271	1287	rBV	323161	690860	22.74%	2.736%
27	12.016	1513	1518	1525	rVB6	6145	12653	0.42%	0.050%
28	13.180	1711	1716	1722	rVB3	7008	10625	0.35%	0.042%
29	13.710	1799	1806	1822	rBV	876209	1287922	42.39%	5.101%
30	13.904	1838	1839	1844	rBV5	2396	3243	0.11%	0.013%
31	13.974	1844	1851	1861	rBV	1133911	1670848	55.00%	6.617%
32	14.280	1897	1903	1913	rBV	665583	961627	31.65%	3.809%
33	14.539	1941	1947	1963	rBV3	33897	109484	3.60%	0.434%
34	14.851	1987	2000	2008	rBV3	15460	48678	1.60%	0.193%
35	15.286	2064	2074	2084	rBV	1434370	2086482	68.68%	8.264%
36	15.421	2090	2097	2111	rBV	421358	622217	20.48%	2.464%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
 Data File : BM044985.D
 Acq On : 07 Apr 2024 00:27
 Operator : MA/JU
 Sample : P2013-01
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0M88

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

37	15.527	2111	2115	2120	rVB6	5699	9145	0.30%	0.036%
38	16.068	2204	2207	2213	rVB7	4630	7439	0.24%	0.029%
39	16.462	2271	2274	2278	rVB6	2743	3981	0.13%	0.016%
40	16.598	2292	2297	2298	rBV4	2182	3112	0.10%	0.012%
41	16.815	2327	2334	2336	rBV8	3892	7487	0.25%	0.030%
42	17.039	2366	2372	2381	rBV	791163	1120513	36.88%	4.438%
43	17.139	2383	2389	2401	rBV	1679596	2359166	77.65%	9.343%
44	17.821	2502	2505	2509	rBV6	2808	4603	0.15%	0.018%
45	17.951	2522	2527	2541	rBV	60035	102664	3.38%	0.407%
46	18.386	2598	2601	2605	rVB5	4941	4724	0.16%	0.019%
47	19.009	2703	2707	2712	rVB3	20844	25927	0.85%	0.103%
48	19.086	2715	2720	2724	rBV3	14682	23050	0.76%	0.091%
49	19.245	2742	2747	2755	rBV4	31449	52716	1.74%	0.209%
50	19.392	2769	2772	2775	rBV5	8395	8439	0.28%	0.033%
51	19.445	2775	2781	2790	rVV	2017882	2719707	89.52%	10.771%
52	19.574	2801	2803	2804	rBV2	4664	3138	0.10%	0.012%
53	21.250	3082	3088	3095	rBV	898609	1267068	41.71%	5.018%
54	23.333	3435	3442	3449	rBV2	1696353	3038028	100.00%	12.032%
55	23.468	3459	3465	3476	rVB	731527	1419105	46.71%	5.620%




Sum of corrected areas: 25249334

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM044985.D
Acq On : 07 Apr 2024 00:27
Operator : MA/JU
Sample : P2013-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0M88

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

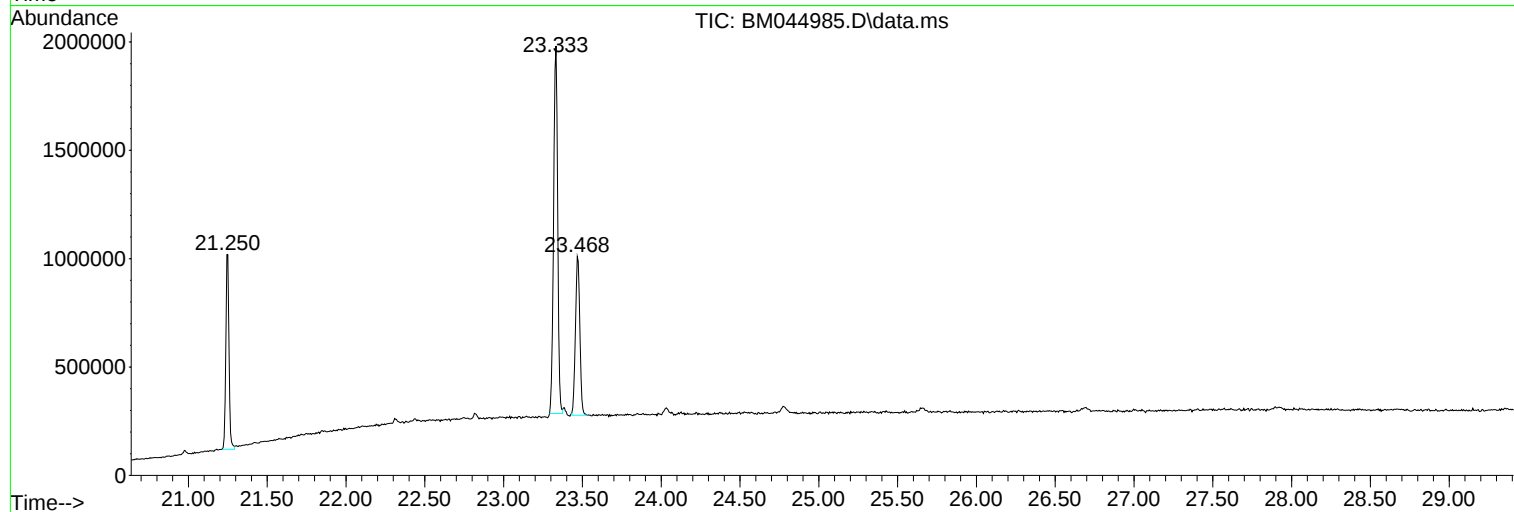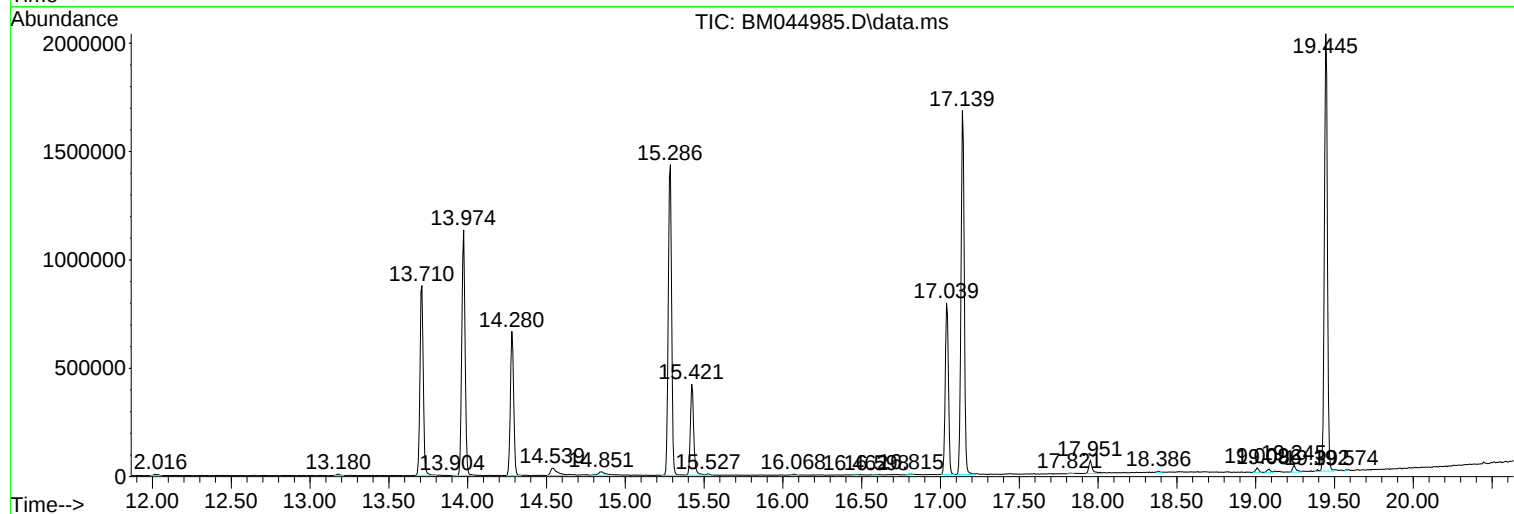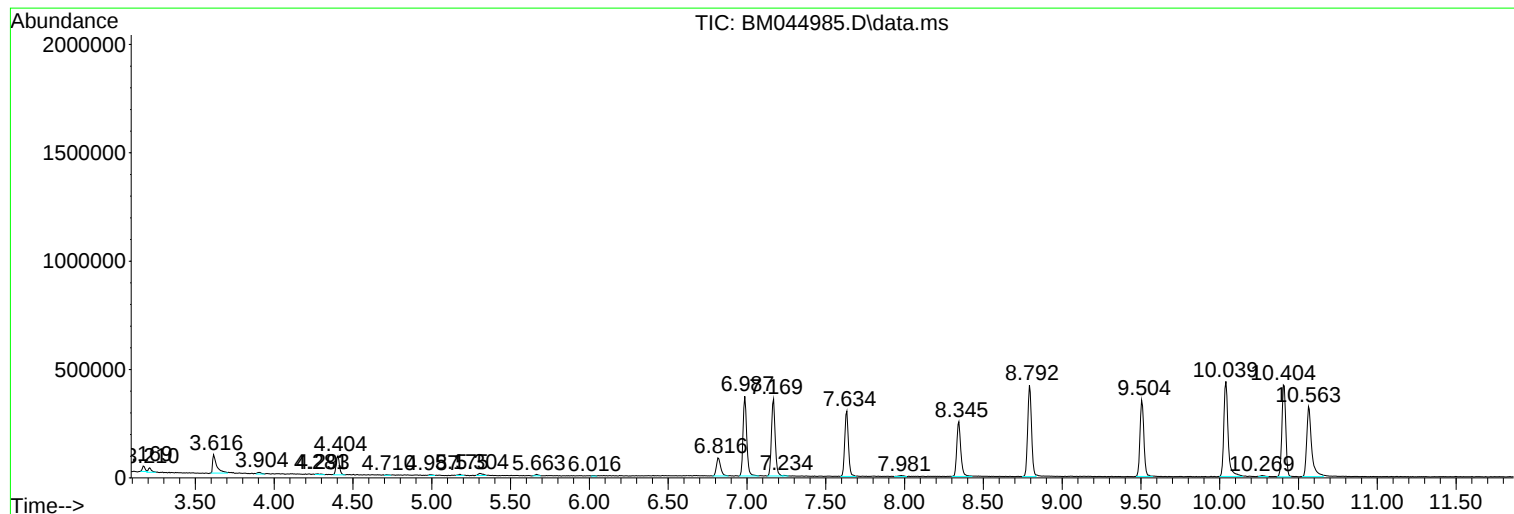

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM044985.D
Acq On : 07 Apr 2024 00:27
Operator : MA/JU
Sample : P2013-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0M88

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM044985.D
Acq On : 07 Apr 2024 00:27
Operator : MA/JU
Sample : P2013-01
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0M88

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc