

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
 Data File : BM044988.D
 Acq On : 07 Apr 2024 02:14
 Operator : MA/JU
 Sample : P2013-04
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EOMB0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044988.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	9	14	30	rVB	415405	648715	19.99%	2.134%
2	3.616	87	90	103	rBV	97386	183069	5.64%	0.602%
3	4.404	218	224	237	rVB	2374688	3244484	100.00%	10.671%
4	5.181	352	356	359	rVB4	4855	7272	0.22%	0.024%
5	5.304	373	377	386	rVB3	13989	28552	0.88%	0.094%
6	5.663	433	438	442	rBV7	6537	11759	0.36%	0.039%
7	5.916	479	481	486	rVB5	2501	3404	0.10%	0.011%
8	6.816	628	634	644	rBV	99977	180590	5.57%	0.594%
9	6.986	656	663	676	rBV	402420	639829	19.72%	2.104%
10	7.169	687	694	705	rBV	395340	651612	20.08%	2.143%
11	7.634	766	773	783	rBV	324830	524705	16.17%	1.726%
12	8.345	887	894	904	rBV	286064	499817	15.41%	1.644%
13	8.792	963	970	982	rBV	457334	788293	24.30%	2.593%
14	8.945	995	996	1002	rVB5	3411	4127	0.13%	0.014%
15	9.504	1085	1091	1103	rBV	387133	664233	20.47%	2.185%
16	10.039	1175	1182	1201	rBV	499549	936497	28.86%	3.080%
17	10.404	1235	1244	1254	rBV	457246	777986	23.98%	2.559%
18	10.563	1263	1271	1292	rBV	411196	850551	26.22%	2.798%
19	12.021	1513	1519	1527	rVB3	7234	15786	0.49%	0.052%
20	12.427	1583	1588	1591	rVB4	1697	3454	0.11%	0.011%
21	13.180	1712	1716	1722	rBV4	3532	4745	0.15%	0.016%
22	13.710	1795	1806	1819	rBV	974431	1405690	43.33%	4.623%
23	13.974	1844	1851	1866	rBV	1241293	1806703	55.69%	5.942%
24	14.280	1895	1903	1911	rBV	681212	990339	30.52%	3.257%
25	14.539	1940	1947	1961	rBV4	35842	116826	3.60%	0.384%
26	14.627	1961	1962	1968	rVB5	3341	5353	0.16%	0.018%
27	14.962	2014	2019	2021	rBV5	2703	3706	0.11%	0.012%
28	15.286	2066	2074	2086	rBV	1515612	2258233	69.60%	7.428%
29	15.421	2090	2097	2112	rBV	379415	575471	17.74%	1.893%
30	15.527	2112	2115	2120	rVB5	5876	8710	0.27%	0.029%
31	16.068	2204	2207	2214	rVB5	4749	6556	0.20%	0.022%
32	16.886	2344	2346	2350	rBV5	2067	3401	0.10%	0.011%
33	17.039	2363	2372	2380	rBV	815448	1136104	35.02%	3.737%
34	17.139	2383	2389	2404	rVB	1781170	2508122	77.30%	8.249%
35	17.327	2418	2421	2424	rBV5	2771	4573	0.14%	0.015%
36	17.456	2438	2443	2445	rVV5	2180	3472	0.11%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM044988.D
Acq On : 07 Apr 2024 02:14
Operator : MA/JU
Sample : P2013-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EOMB0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Title : SVOA CALIBRATION

37	17.950	2522	2527	2536	rBV3	26062	39581	1.22%	0.130%
38	18.339	2590	2593	2596	rVB5	2408	3335	0.10%	0.011%
39	18.386	2597	2601	2605	rBV6	4023	6283	0.19%	0.021%
40	18.780	2665	2668	2671	rBV5	2413	3628	0.11%	0.012%
41	19.009	2703	2707	2712	rVB4	22287	32331	1.00%	0.106%
42	19.080	2712	2719	2724	rBV	20876	34649	1.07%	0.114%
43	19.245	2743	2747	2751	rBV5	14033	18122	0.56%	0.060%
44	19.397	2770	2773	2775	rBV4	6113	5592	0.17%	0.018%
45	19.445	2775	2781	2790	rBV	2160593	2871736	88.51%	9.445%
46	21.244	3082	3087	3093	rBV	953161	1256508	38.73%	4.133%
47	23.327	3435	3441	3448	rBV	1808466	3187638	98.25%	10.484%
48	23.468	3459	3465	3476	rVB	748706	1441370	44.43%	4.741%




Sum of corrected areas: 30403512

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM044988.D
Acq On : 07 Apr 2024 02:14
Operator : MA/JU
Sample : P2013-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EOMB0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

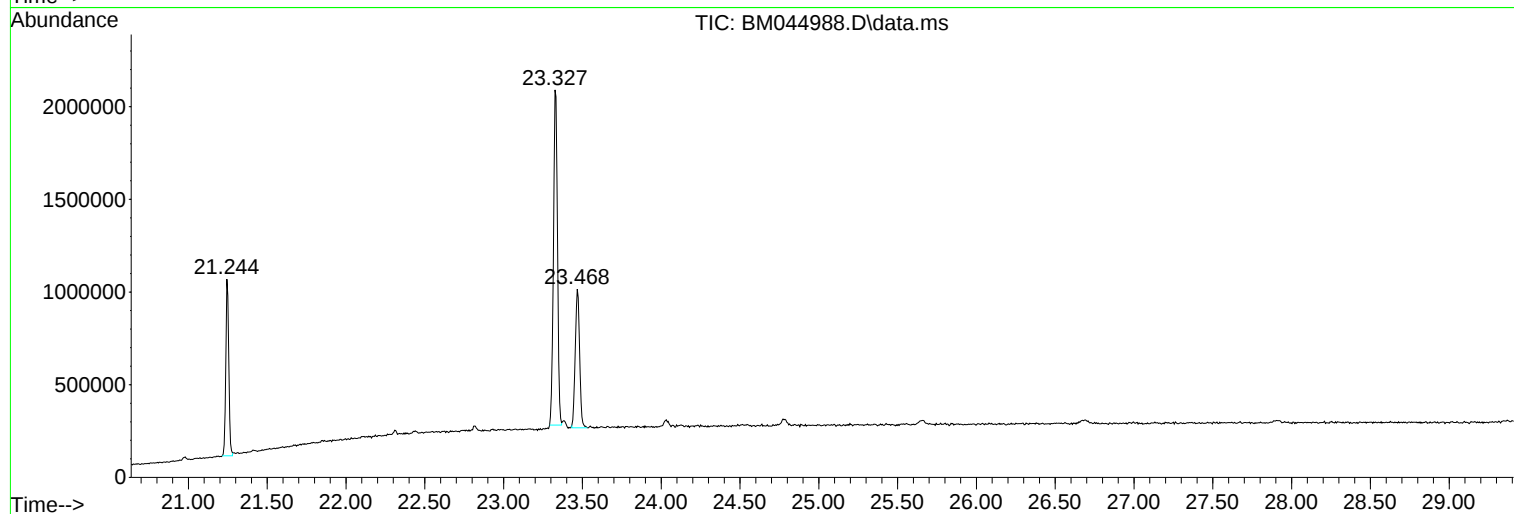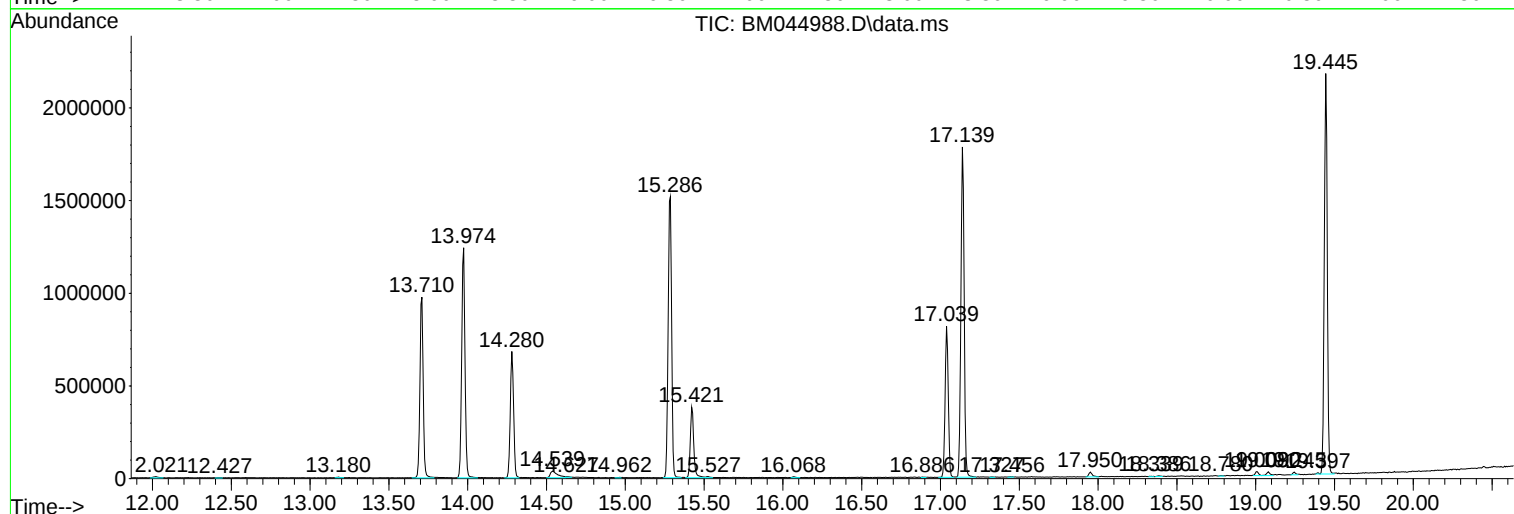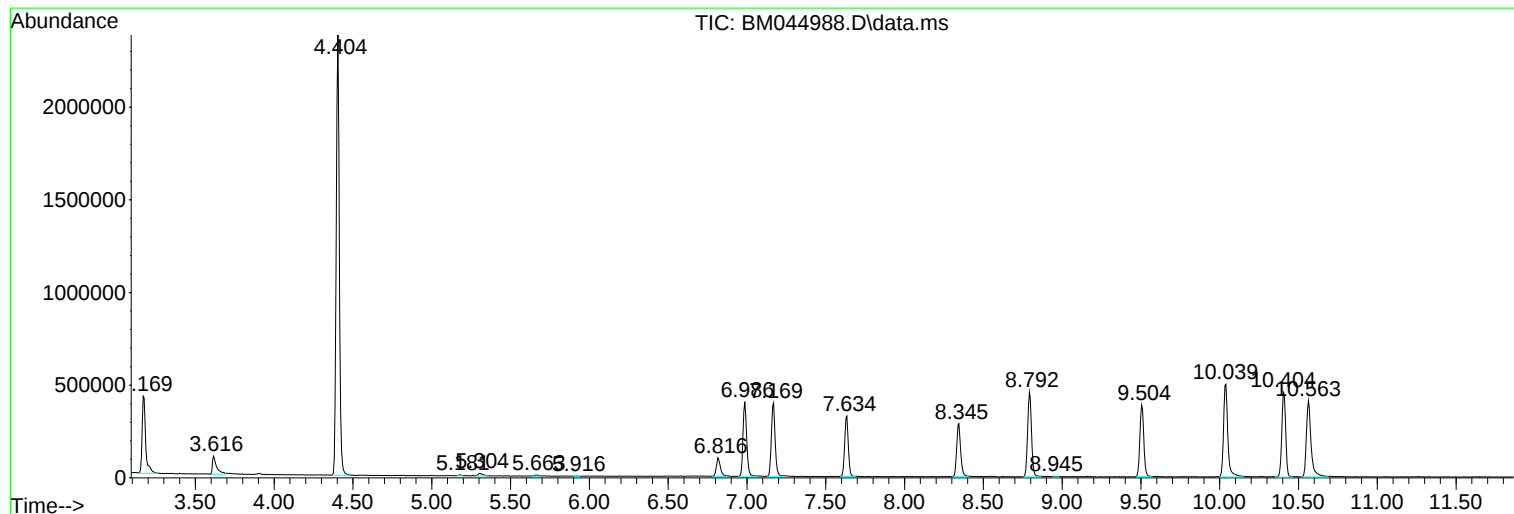

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM044988.D
Acq On : 07 Apr 2024 02:14
Operator : MA/JU
Sample : P2013-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MB0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM040624\
Data File : BM044988.D
Acq On : 07 Apr 2024 02:14
Operator : MA/JU
Sample : P2013-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0MB0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM040524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc